

Sample Name : Peptide YY (PYY), human  
 Cat No. : RP10355  
 Lot No. : E4707219I  
 Time Processed : 3:21:51 PM  
 Month-Day-Year Processed : 10/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

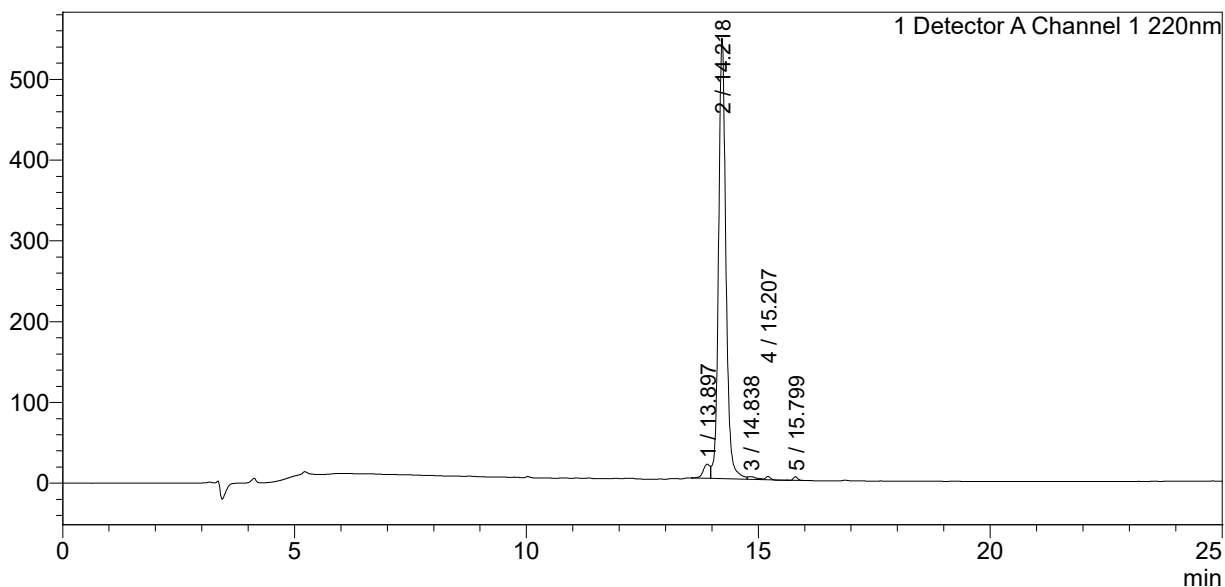

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.897	184394	17598	2.913
2	14.218	6035735	545668	95.337
3	14.838	45373	3520	0.717
4	15.207	32649	4415	0.516
5	15.799	32808	4771	0.518
Total		6330960	575972	100.000