

Sample Name :AngiotensinII.human  
 Cat No.: RP11257  
 Lot No.: PE1381811  
 Time Processed:13:57:53  
 Month-Day-Year Processed:11/29/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

### <Chromatogram>

mV

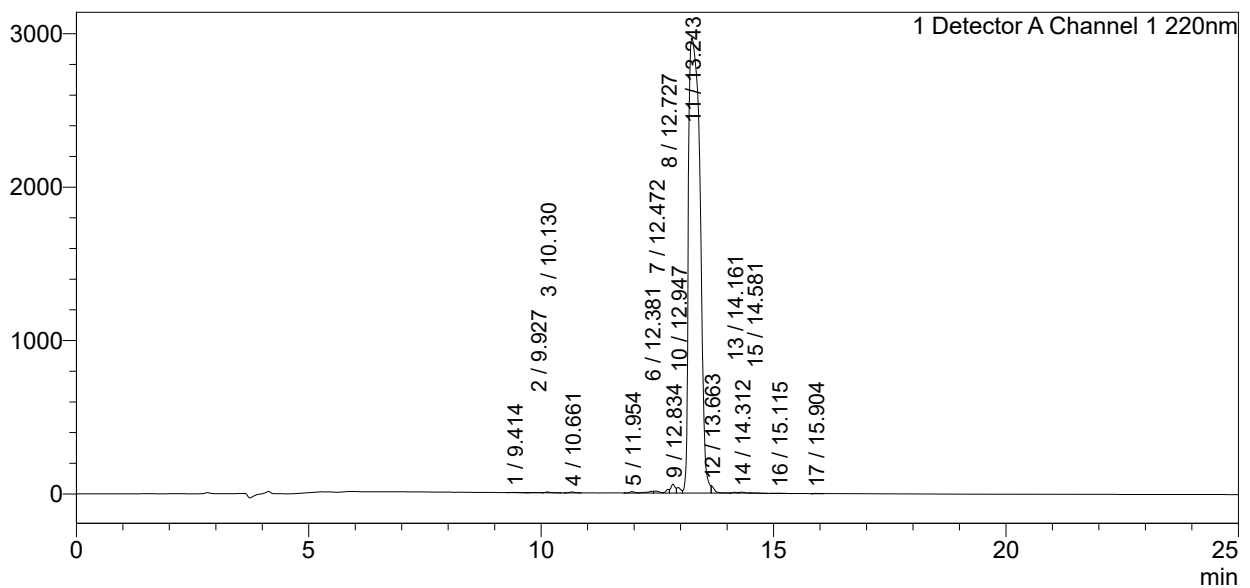

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.414	14592	1688	0.028
2	9.927	9237	879	0.018
3	10.130	30644	5105	0.059
4	10.661	43078	5862	0.083
5	11.954	64953	9159	0.125
6	12.381	108851	11525	0.209
7	12.472	96969	12483	0.186
8	12.727	119735	23603	0.230
9	12.834	371835	57876	0.715
10	12.947	216563	35493	0.416
11	13.243	50599458	2967089	97.300
12	13.663	210720	47609	0.405
13	14.161	31516	5488	0.061
14	14.312	43208	6268	0.083
15	14.581	14042	1299	0.027

Peak#	Ret. Time	Area	Height	Area%
16	15.115	16903	1475	0.033
17	15.904	11145	1874	0.021
Total		52003448	3194775	100.000