

Sample Name: CLIP (86-100)
 Cat No. :RP20279
 Lot No. :E6889620H
 Time Processed: 8:54:52 AM
 Month-Day-Year Processed :08/06/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

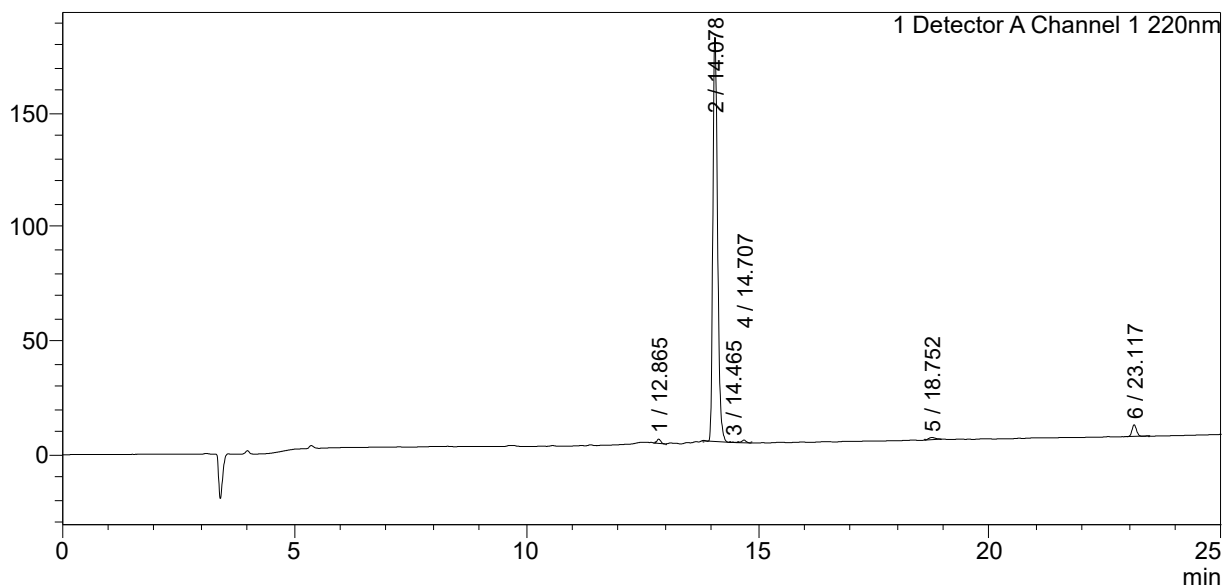

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.865	9980	1838	0.759
2	14.078	1250599	177573	95.133
3	14.465	1299	191	0.099
4	14.707	8582	1228	0.653
5	18.752	9252	937	0.704
6	23.117	34868	5162	2.652
Total		1314580	186929	100.000