

Sample Name : β -Amyloid (22-35)
 Cat. No. :RP20130
 Lot. No. :PE8821902
 Time Processed : 10:52:00
 Month-Day-Year
 Processed :03/02/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

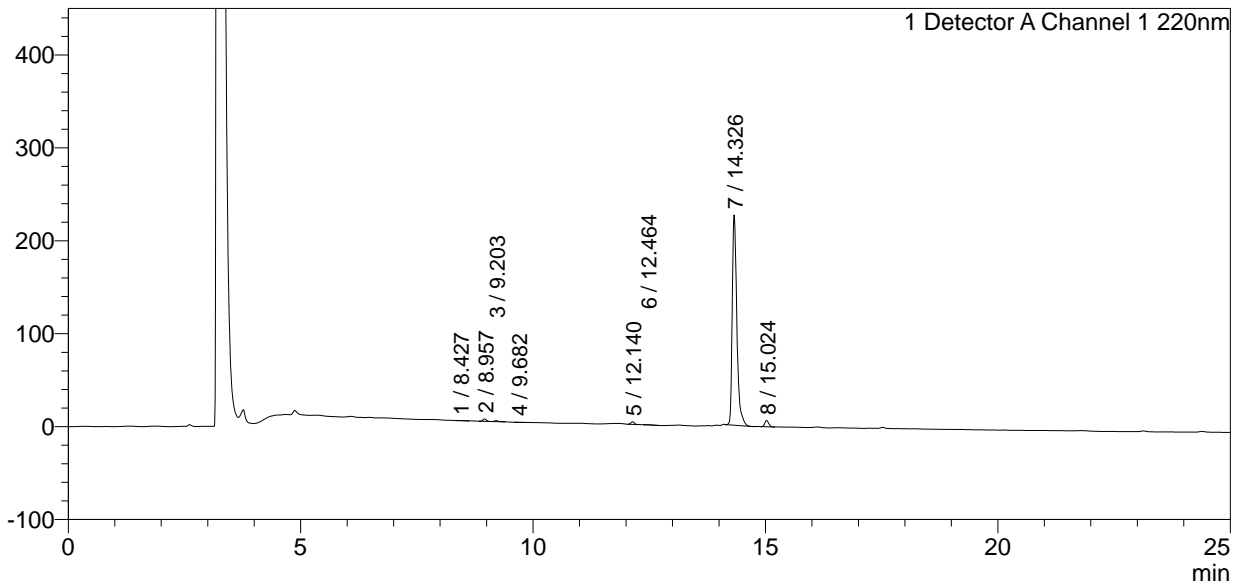

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.427	1160	133	0.071
2	8.957	12965	2556	0.796
3	9.203	5796	1036	0.356
4	9.682	1162	120	0.071
5	12.140	14942	2828	0.917
6	12.464	2585	303	0.159
7	14.326	1551416	226243	95.249
8	15.024	38781	6717	2.381
Total		1628808	239935	100.000