

Sample Name : [Met5]-Enkephalin, amide
 Cat No. : RP10887
 Lot No. : E4771219I
 Time Processed : 6:34:12 AM
 Month-Day-Year Processed : 09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

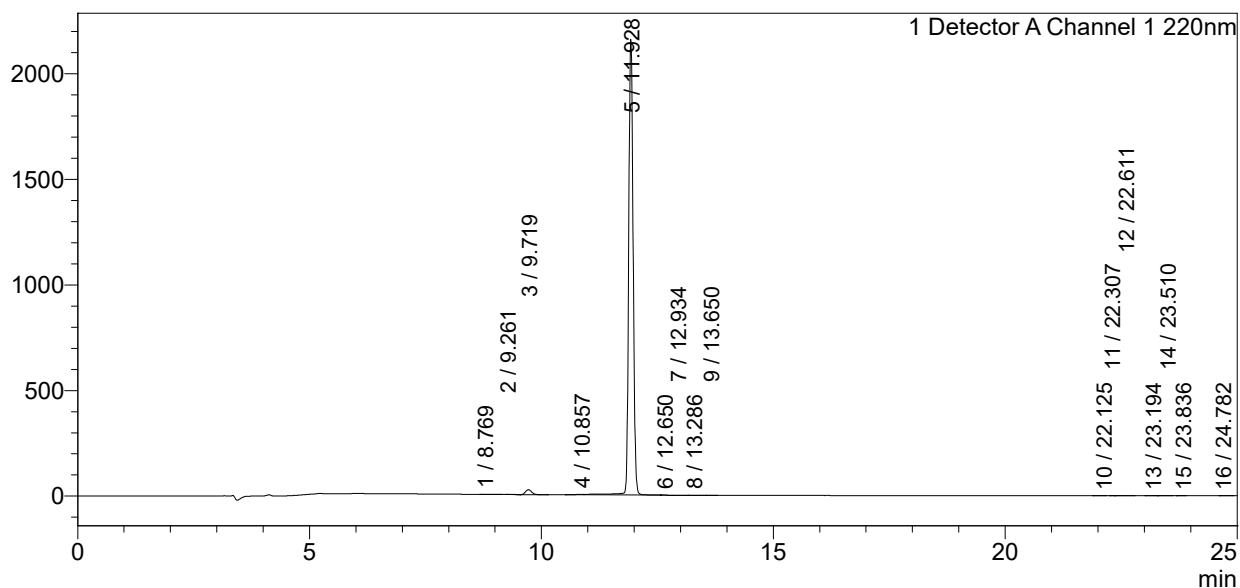

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.769	3426	403	0.023
2	9.261	1347	55	0.009
3	9.719	216121	23318	1.464
4	10.857	31217	2558	0.212
5	11.928	14482140	2158989	98.135
6	12.650	3262	612	0.022
7	12.934	2362	304	0.016
8	13.286	1825	209	0.012
9	13.650	3219	555	0.022
10	22.125	1520	170	0.010
11	22.307	1027	166	0.007
12	22.611	3950	173	0.027
13	23.194	1381	120	0.009
14	23.510	2125	124	0.014
15	23.836	1135	109	0.008

Peak#	Ret. Time	Area	Height	Area%
16	24.782	1376	123	0.009
Total		14757432	2187990	100.000