

Sample Name :Systemin

Cat No. : RP10622

Lot No. : PE5401808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command         | Value |
|-------|------------|-----------------|-------|
| 0.01  | Pumps      | Solvent B Conc. | 5     |
| 25.00 | Pumps      | Solvent B Conc. | 65    |
| 25.01 | Pumps      | Solvent B Conc. | 95    |
| 27.00 | Pumps      | Solvent B Conc. | 95    |
| 27.01 | Pumps      | Solvent B Conc. | 5     |
| 33.00 | Pumps      | Solvent B Conc. | 5     |
| 33.01 | Controller | Stop            |       |


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

### <Chromatogram>

mV

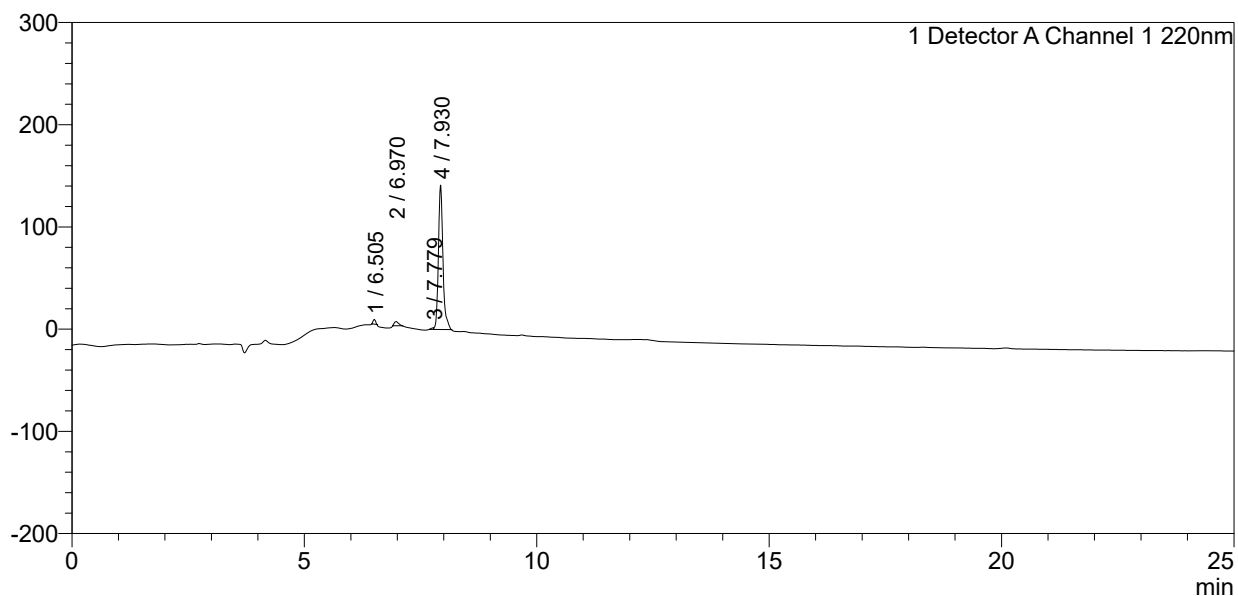

### <Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area    | Height | Area%   |
|-------|-----------|---------|--------|---------|
| 1     | 6.505     | 17025   | 4609   | 1.688   |
| 2     | 6.970     | 26950   | 4136   | 2.671   |
| 3     | 7.779     | 6259    | 1462   | 0.620   |
| 4     | 7.930     | 958595  | 141258 | 95.021  |
| Total |           | 1008829 | 151465 | 100.000 |