

Sample Name :InsB 9-23
 Cat. No. :RP20391
 Lot. No. :PE6131702

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

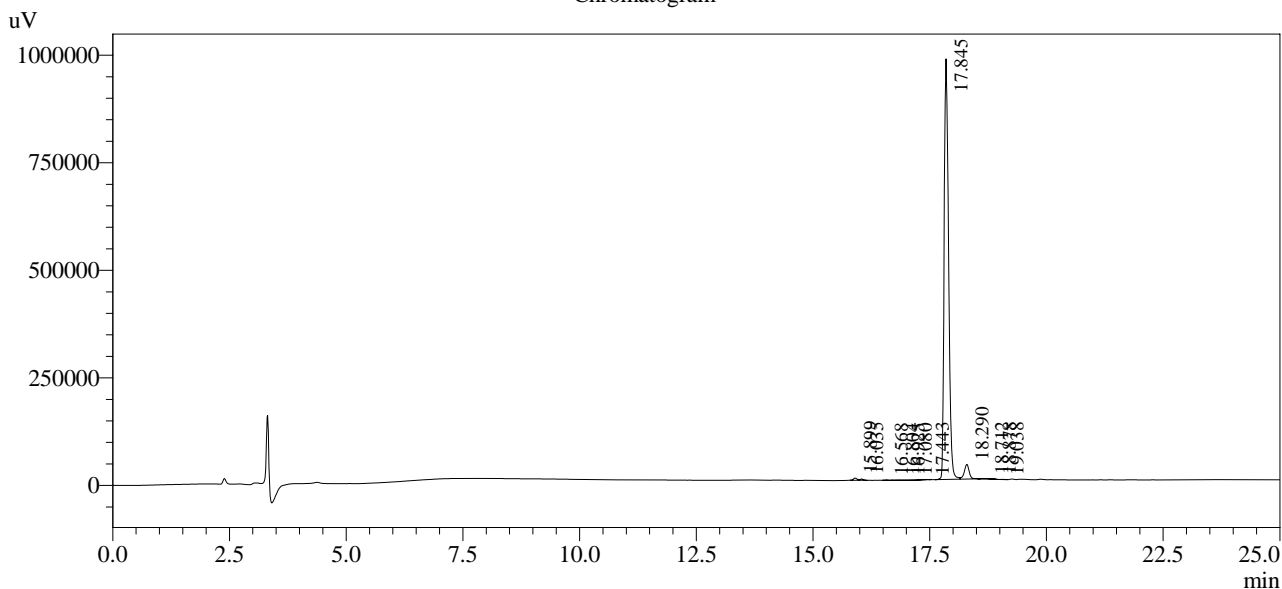

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.899	27190	5029	0.400
2	16.035	14597	2836	0.215
3	16.568	3192	675	0.047
4	16.804	2549	461	0.038
5	16.925	3698	697	0.054
6	17.080	3000	538	0.044
7	17.443	7153	768	0.105
8	17.845	6471298	977793	95.230
9	18.290	248981	34208	3.664
10	18.712	6643	760	0.098
11	18.878	4931	1033	0.073
12	19.038	2179	396	0.032
Total		6795411	1025194	100.000