


Mass Spectrum

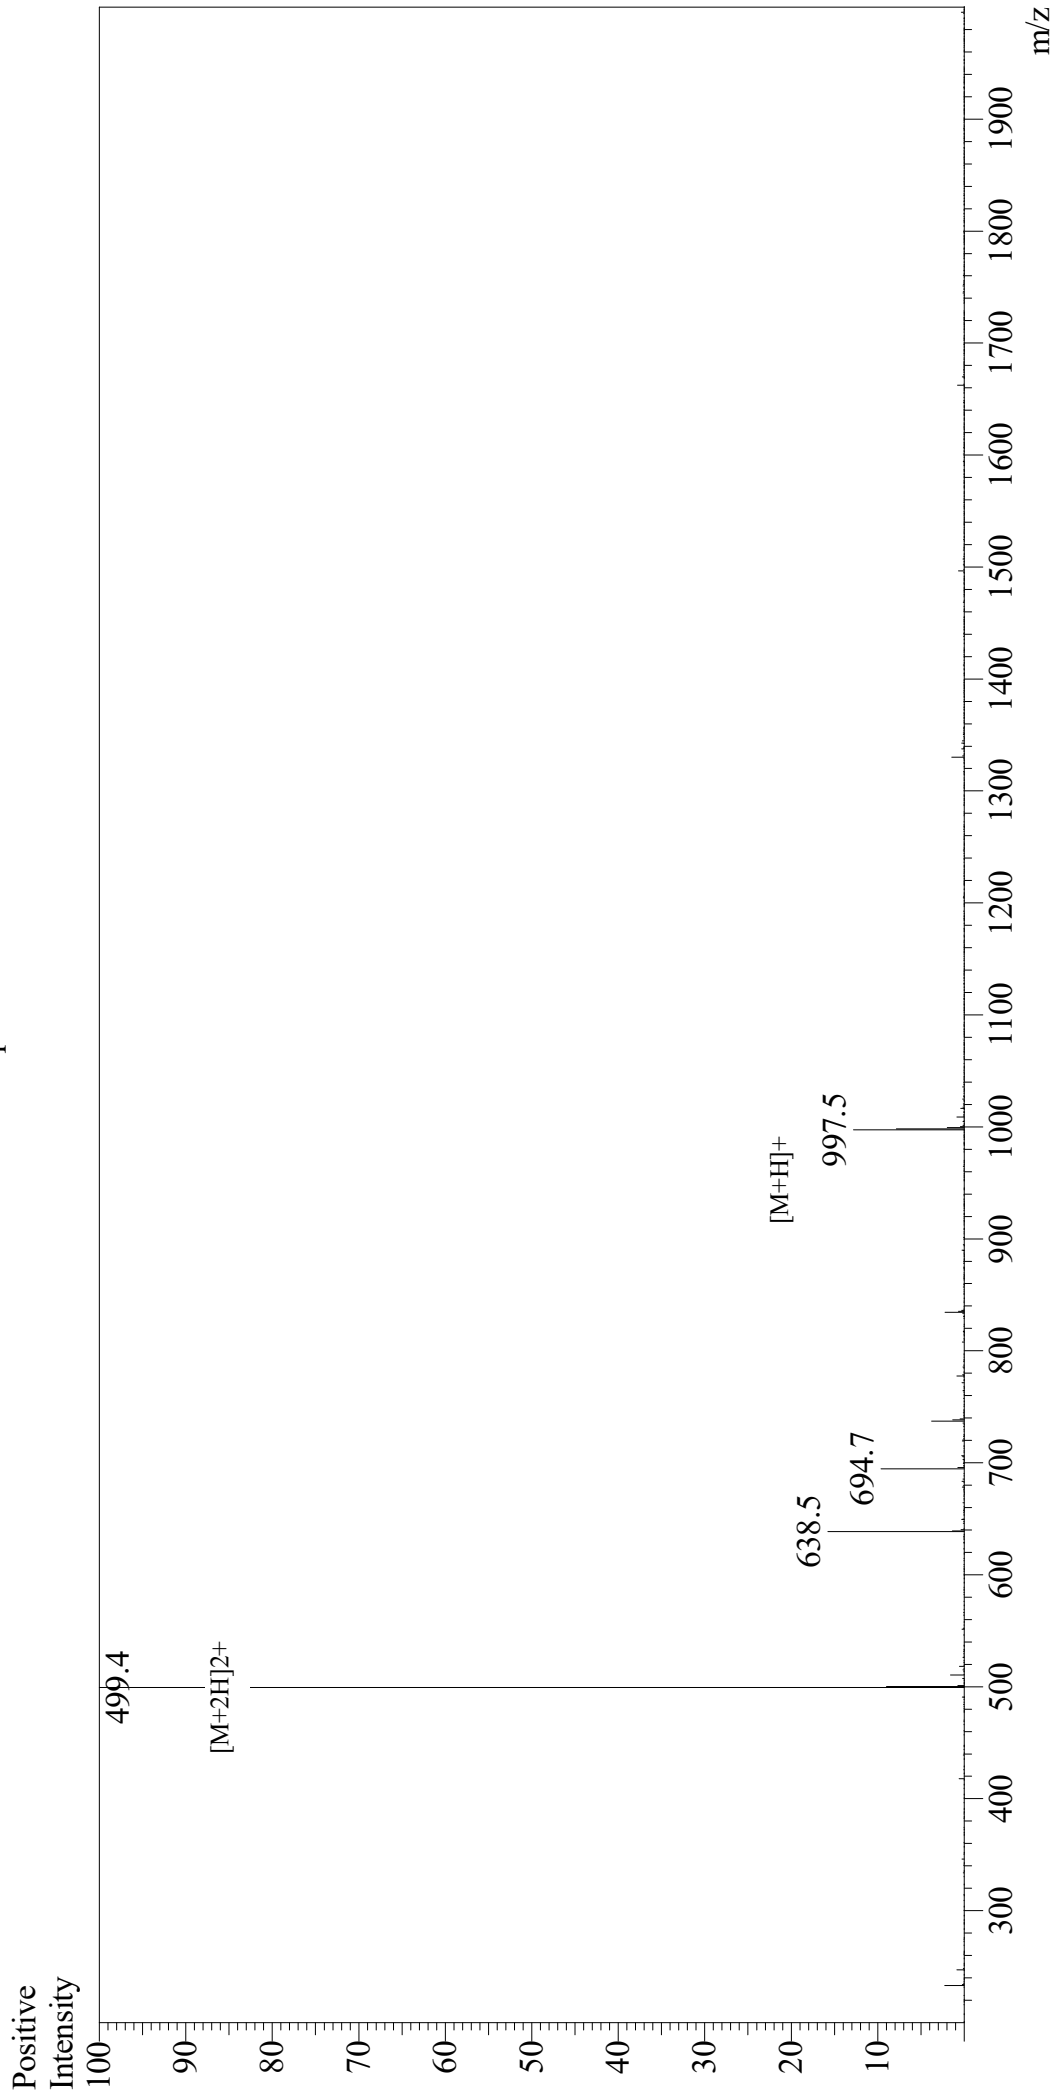

Sample Information

User : Gary
Month-Day Processed : 09/21/19
Time Processed : 12:49:43 PM
Injection Volume : 0.3
Sample Name : Hemorphin-7
Cat No. : RP17312
Lot No. : E4904919I
Theoretical MW : 997.11
Observed MW : 996.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH