

Sample Name :YRGDS Fibronectin Fragment
 Cat. No. : RP20476 Lot. No. : PE2311712

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

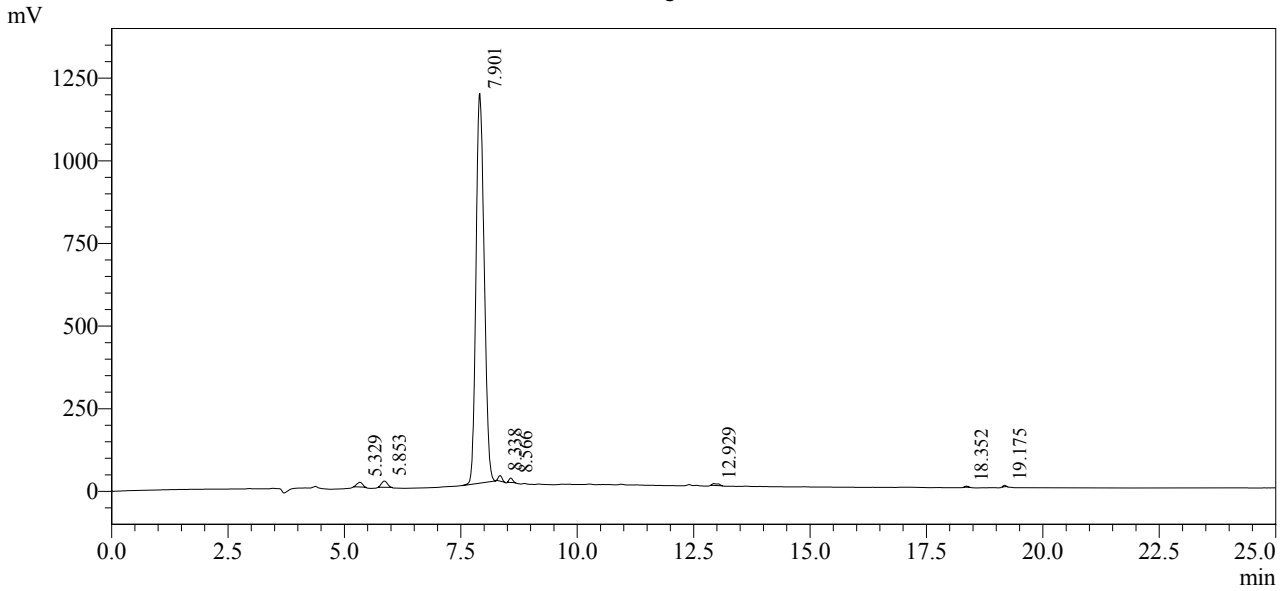

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.329	120542	14347	0.807
2	5.853	168435	19110	1.127
3	7.901	14400980	1179071	96.394
4	8.338	91739	16466	0.614
5	8.566	72206	13221	0.483
6	12.929	55610	5667	0.372
7	18.352	13079	3153	0.088
8	19.175	17174	4367	0.115
Total		14939764	1255403	100.000