

Sample Name : LAH4
 Cat No : RP20096
 Lot No : E6723121D
 Time Processed : 9:43:17 PM
 Month-Day-Year Processed : 04/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

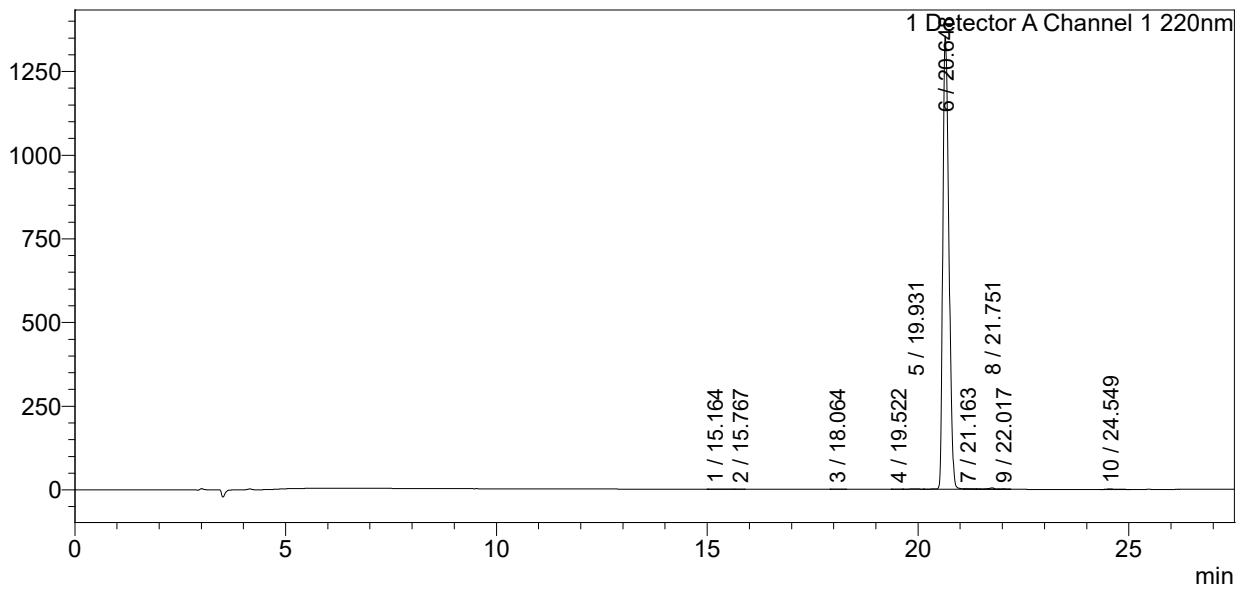

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.164	5977	446	0.044
2	15.767	1638	252	0.012
3	18.064	2801	367	0.020
4	19.522	2433	311	0.018
5	19.931	23691	1660	0.173
6	20.648	13615020	1352860	99.197
7	21.163	4619	604	0.034
8	21.751	35924	3971	0.262
9	22.017	7060	937	0.051
10	24.549	26094	1509	0.190
Total		13725256	1362917	100.000