

Sample Name : Biotin-TAT (47-57)
 Cat. No. : RP20408
 Lot. No. : PE8741807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

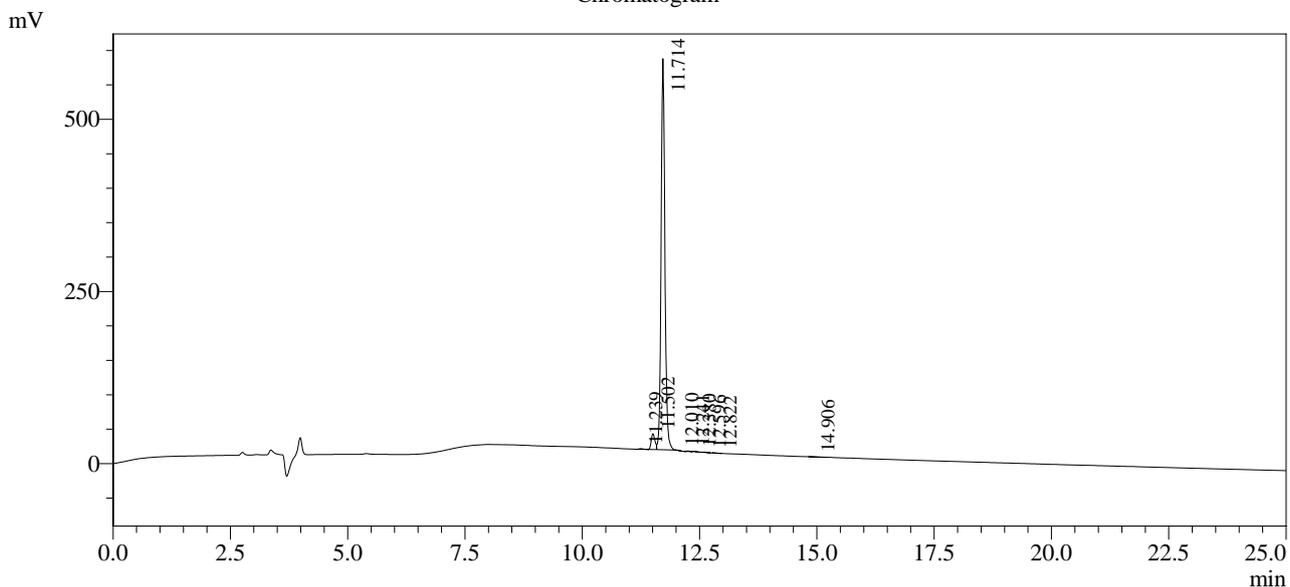

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.239	5372	918	0.160
2	11.502	126931	23003	3.776
3	11.714	3213967	568115	95.614
4	12.010	1553	456	0.046
5	12.241	2411	623	0.072
6	12.380	3789	769	0.113
7	12.596	2810	519	0.084
8	12.822	1396	272	0.042
9	14.906	3160	214	0.094
Total		3361388	594890	100.000