


# Mass Spectrum

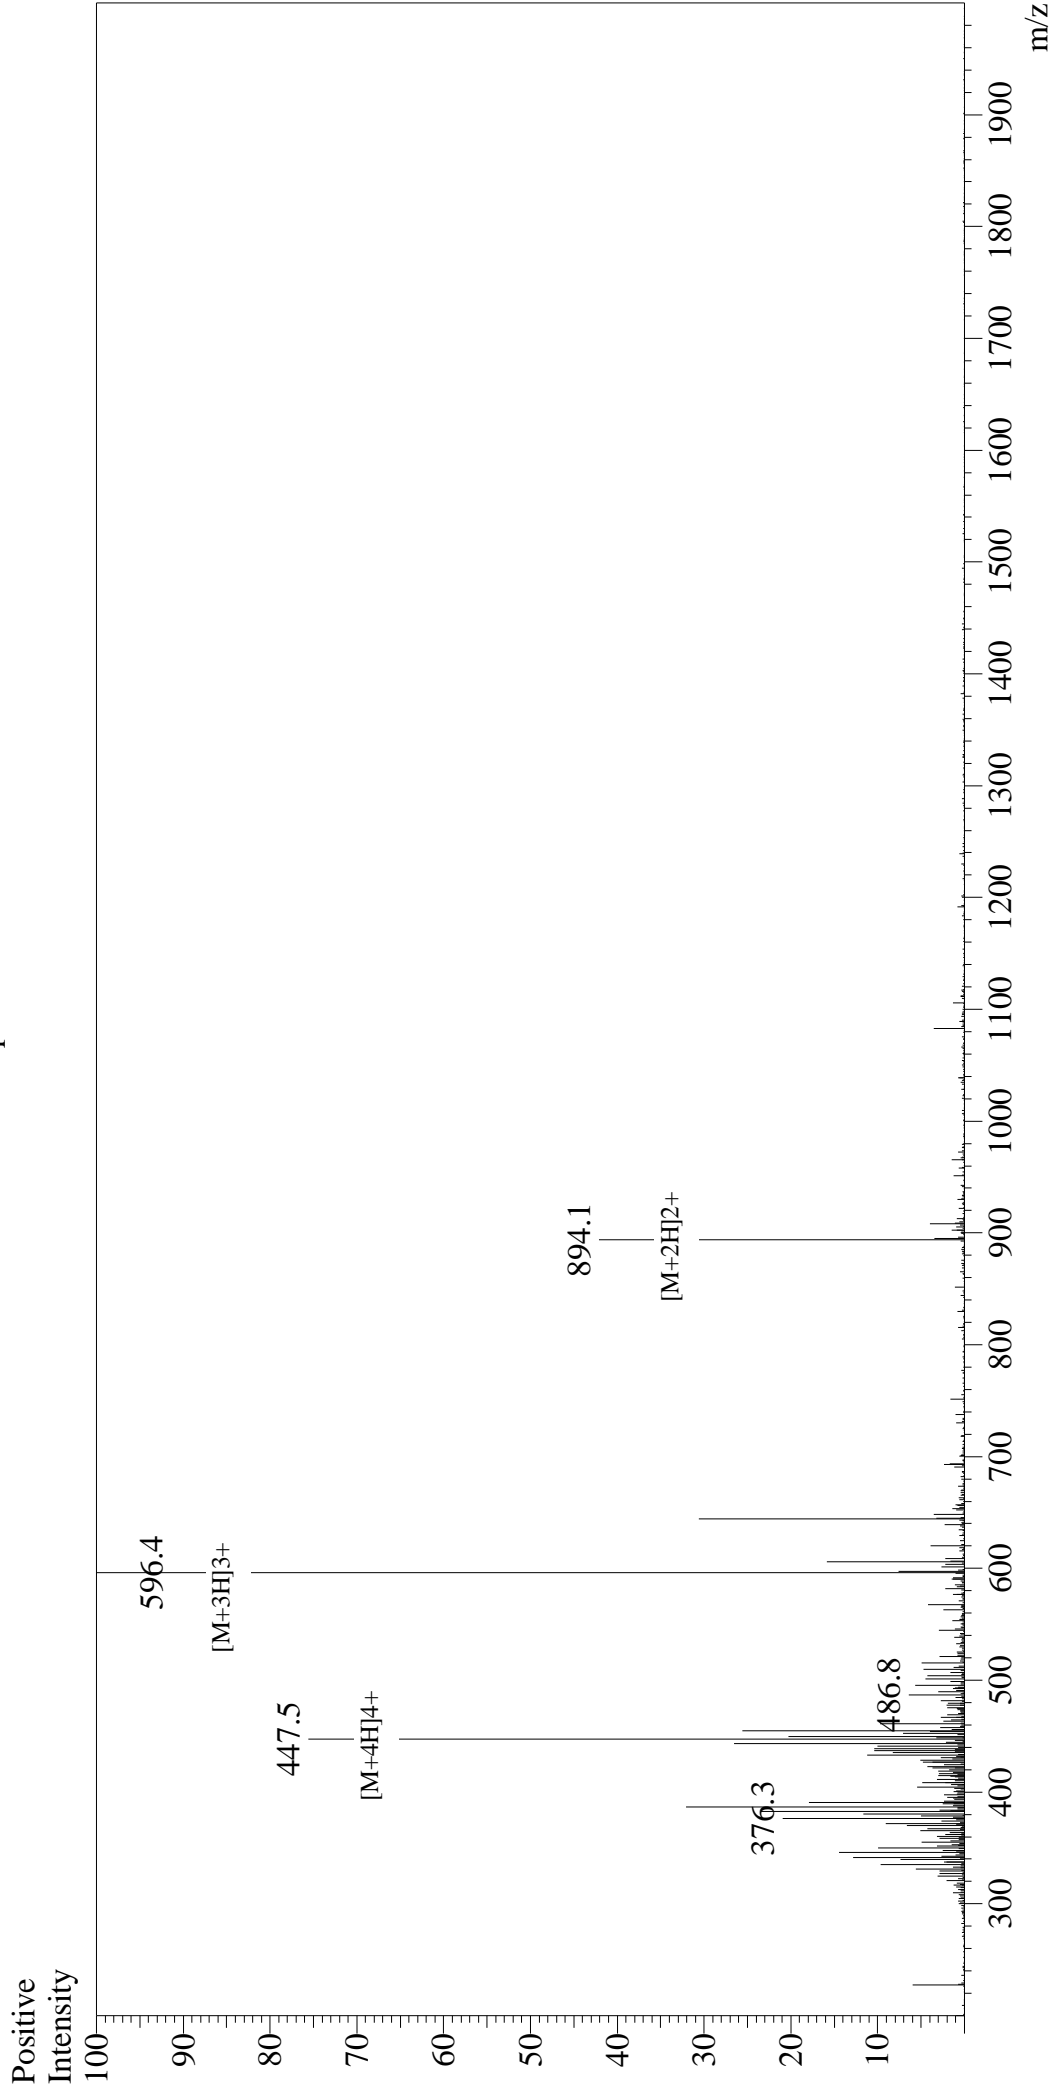

## Sample Information

User : Gary  
Month-Day Processed : 08/03/18  
Time Processed : 10:01:53  
Injection Volume : 0.2  
Sample Name : Biotin-TAT (47-57)  
Cat No. : RP20408  
Lot No. : PE8741807  
Theoretical MW : 1786.20  
Observed MW : 1786.2

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250°C  
Block Temp : 200°C

Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH