

Sample Name :C-telopeptide
 Cat No :RP10566
 Lot No :E9797120J
 Time Processed :19:15:03
 Month-Day-Year Processed :11/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

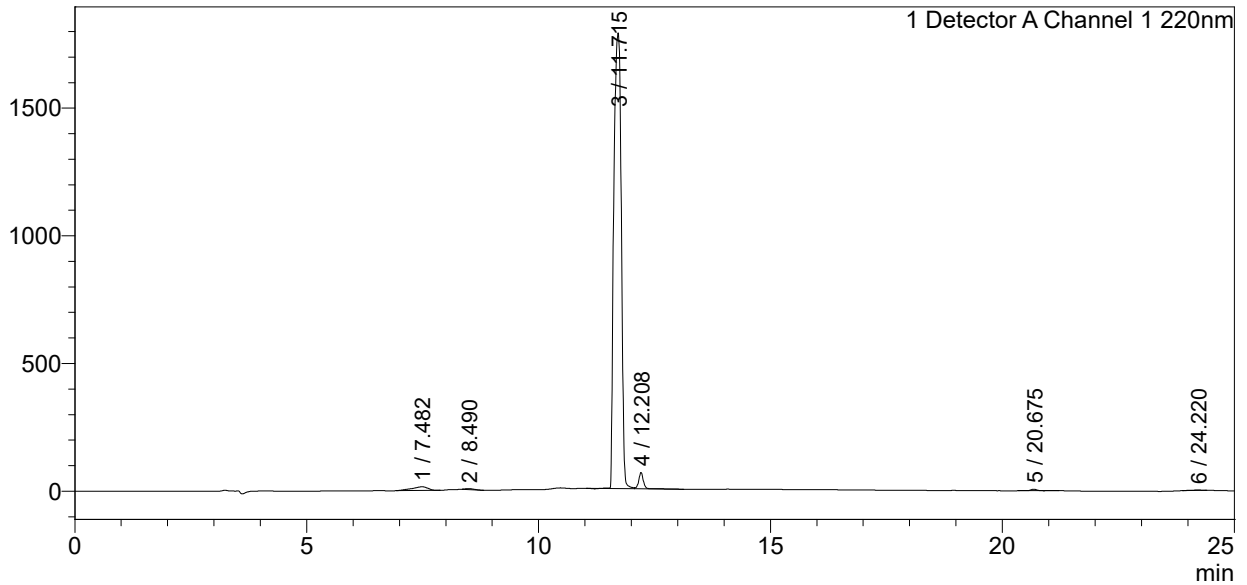

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.482	358225	14643	1.733
2	8.490	41437	3378	0.200
3	11.715	19734860	1785294	95.485
4	12.208	459418	64370	2.223
5	20.675	51492	5935	0.249
6	24.220	22526	1046	0.109
Total		20667957	1874666	100.000