

Sample Name : Biotin-TAT (47-57)
 Cat No.: RP20408
 Lot No.: E5494120A
 Time Processed : 11:01:35
 Month-Day-Year Processed : 01/25/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010014

<Chromatogram>

mV

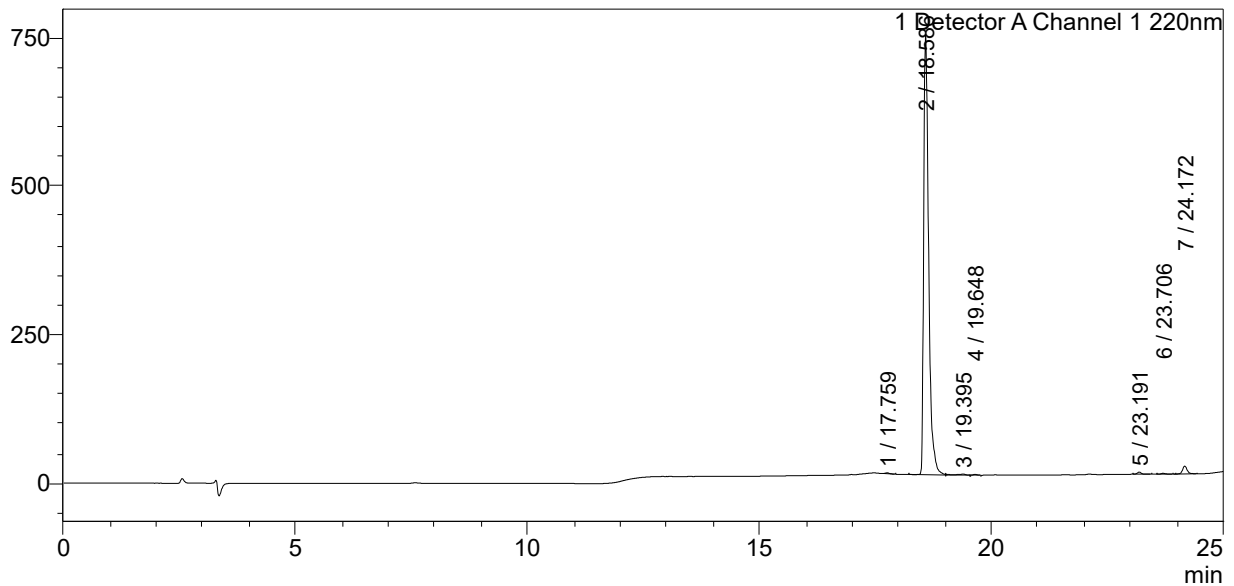

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.759	8041	1494	0.142
2	18.586	5501649	740401	97.294
3	19.395	21643	1785	0.383
4	19.648	6873	1353	0.122
5	23.191	19224	3473	0.340
6	23.706	8844	1438	0.156
7	24.172	88376	13100	1.563
Total		5654651	763043	100.000