

Sample Name :DYKDDDDK Peptide  
 Cat No. :RP10586  
 Lot No. :E8066521C  
 Time Processed :1:54:15 PM  
 Month-Day-Year Processed :03/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
25.00	Pumps	B.Conc	50
25.01	Pumps	B.Conc	95
30.00	Pumps	B.Conc	95
30.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

<Chromatogram>

mV

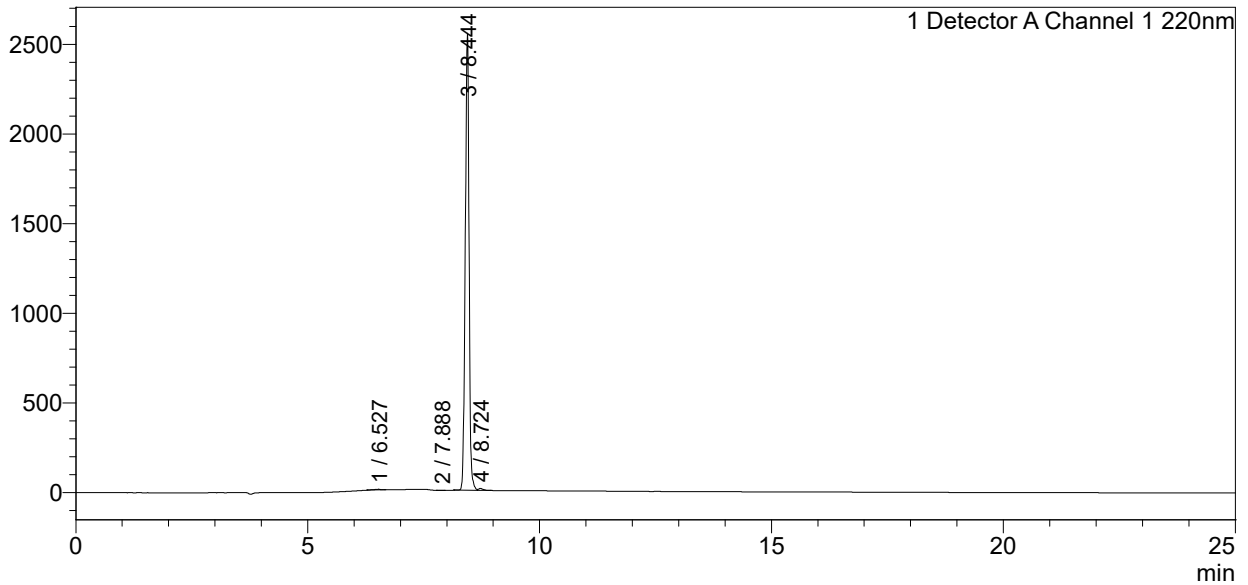

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.527	37769	3897	0.260
2	7.888	2896	842	0.020
3	8.444	14424749	2548665	99.224
4	8.724	72205	11221	0.497
Total		14537618	2564625	100.000