Mass Spectrum

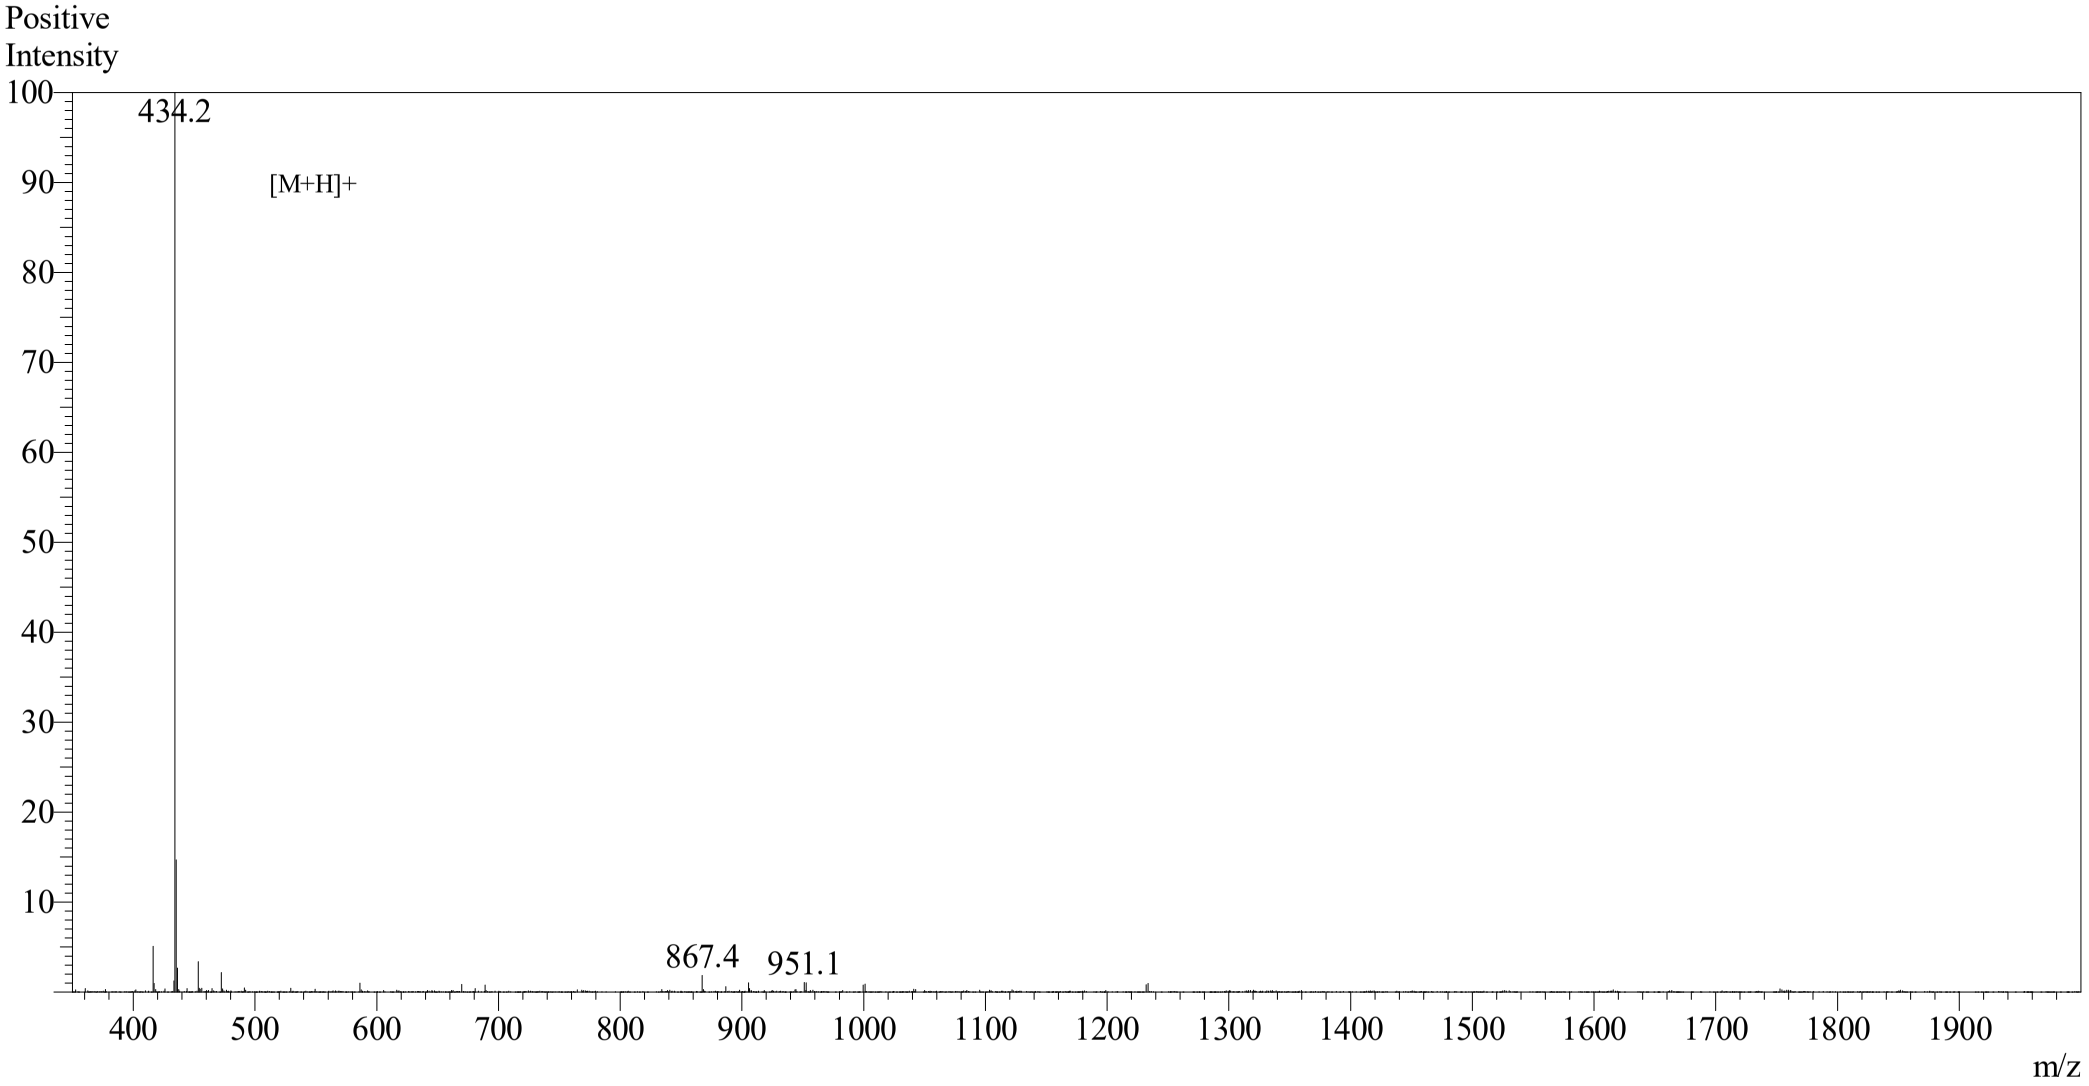

Sample Information

Month-Day Processed :	05/23/21
Time Processed :	12:37:12
Injection Volume :	0.2
Sample Name :	Arg-Gly-Asp-Ser
Cat No. :	RP10861
Lot No. :	E0663221E
Theoretical MW :	433.42
Observed MW :	433.2

Interface	:ESI
Nebulizing Gas Flow	:1.5L/min
CDL Temp	:250
Block Temp	:200

Equipment	: GK11010007
Interface Bias	: +4.5 kV
Drying Gas Flow	:5 L/min
T.Flow	:0.2 ml/min
B.conc	:50%H2O/50%MeOH