

Sample Name :Cecropin B  
 Cat. No. : RP11225  
 Lot. No. : PE8431902  
 Time Processed : 14:48:28  
 Month-Day-Year Processed : 03/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
45.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

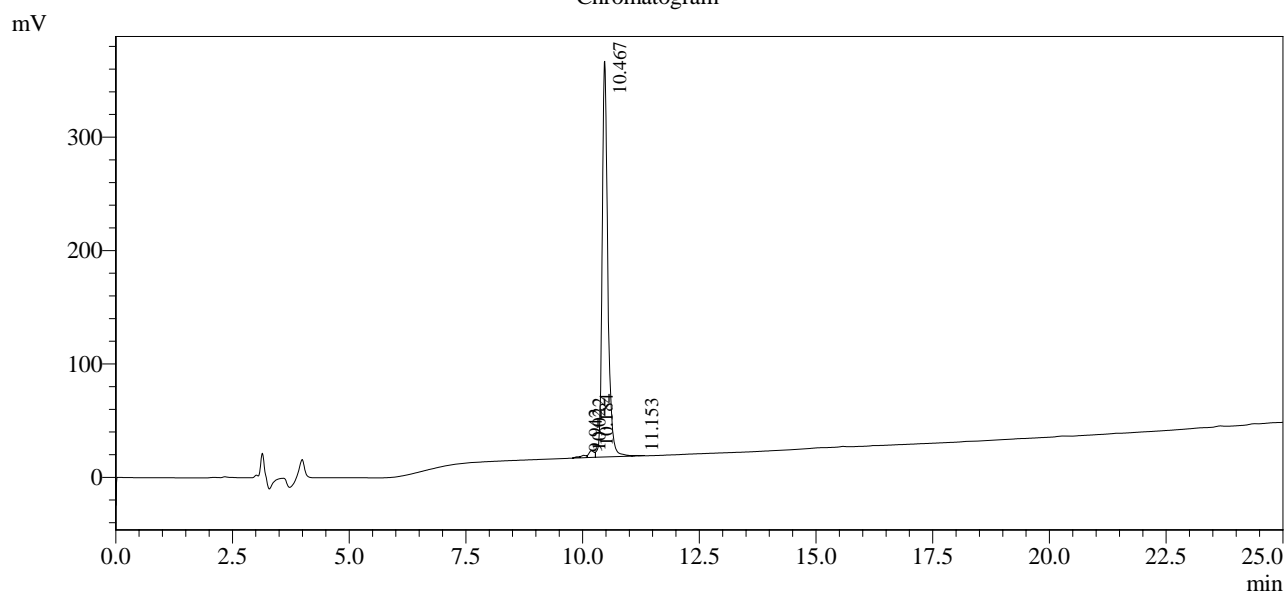

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.942	7665	1027	0.257
2	10.022	15775	2074	0.528
3	10.184	48481	5965	1.624
4	10.467	2909679	349032	97.475
5	11.153	3452	375	0.116
Total		2985051	358473	100.000