

Sample Information

Sample Name :Bradykinin
 Cat. No :RP11129
 Lot. No. :PE3421801

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

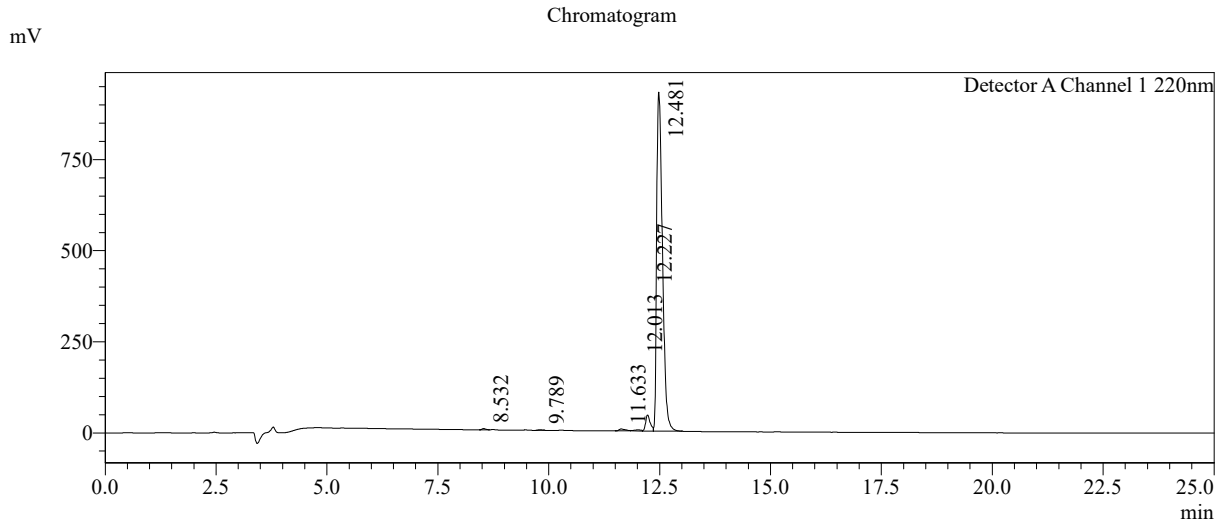

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	8.532	3608	20149	0.365	0.227
2	9.789	1480	9269	0.150	0.105
3	11.633	5343	54031	0.541	0.609
4	12.013	3505	36072	0.355	0.407
5	12.227	43857	314647	4.440	3.548
6	12.481	929976	8433200	94.149	95.104
Total		987770	8867368	100.000	100.000