

Sample Name :Melanin Concentrating Hormone, salmon  
 Cat No. :RP10662  
 Lot No. :PE5811903  
 Time Processed :17:01:20  
 Month-Day-Year Processed :03/31/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ17010508

<Chromatogram>

mV

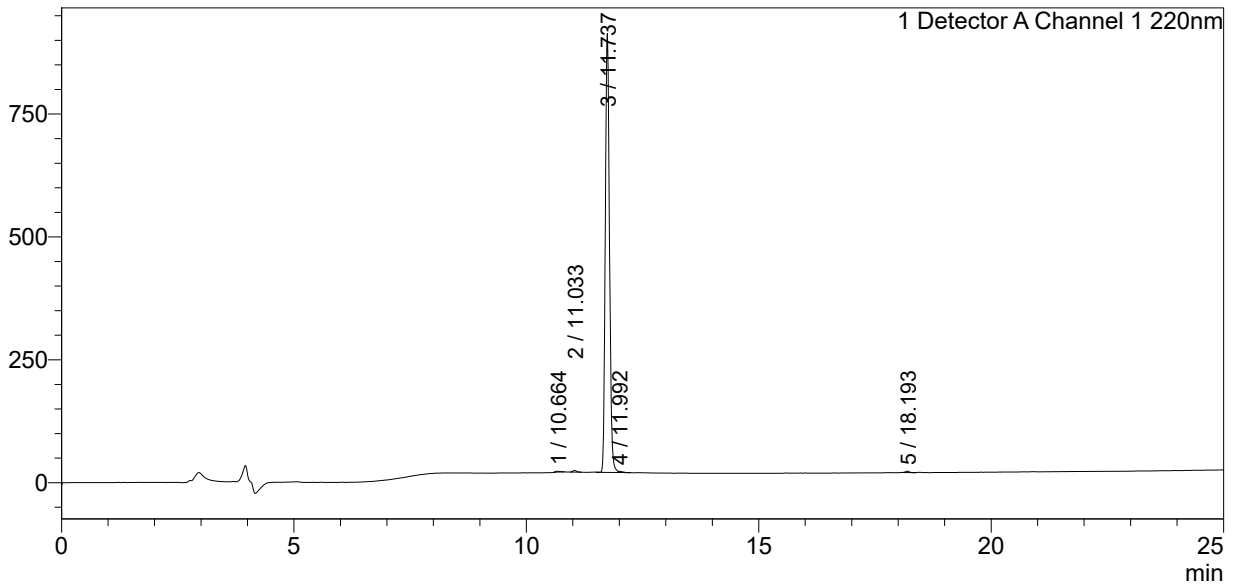

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.664	10732	1758	0.189
2	11.033	18212	3243	0.321
3	11.737	5612420	893033	98.938
4	11.992	14949	2312	0.264
5	18.193	16372	2743	0.289
Total		5672685	903089	100.000