

Sample Name : Peptide YY (PYY), human  
 Cat No.: RP10355  
 Lot No.: E0317820B  
 Time Processed :15:54:41  
 Month-Day-Year Processed :02/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

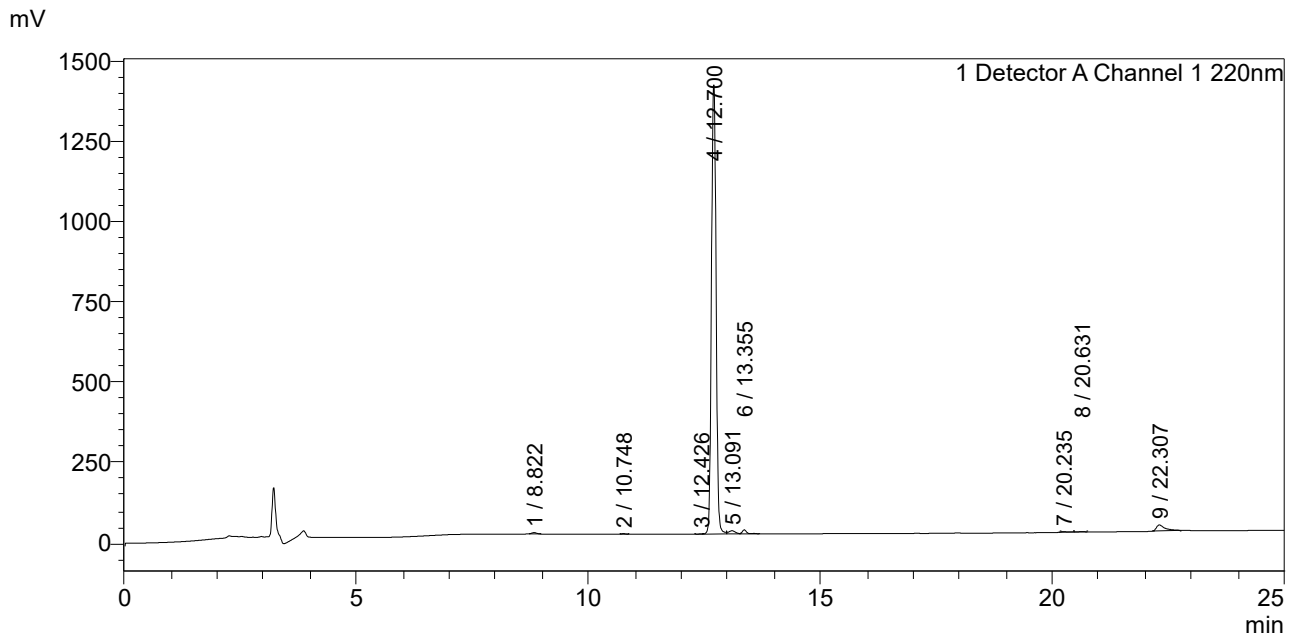

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.822	27927	3978	0.275
2	10.748	8151	1722	0.080
3	12.426	2089	373	0.021
4	12.700	9666703	1399792	95.221
5	13.091	101179	10049	0.997
6	13.355	87262	12789	0.860
7	20.235	17585	1958	0.173
8	20.631	9605	1350	0.095
9	22.307	231400	18892	2.279
Total		10151902	1450903	100.000