

Sample Name : MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E8670320B
 Time Processed :23:49:10
 Month-Day-Year Processed :03/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

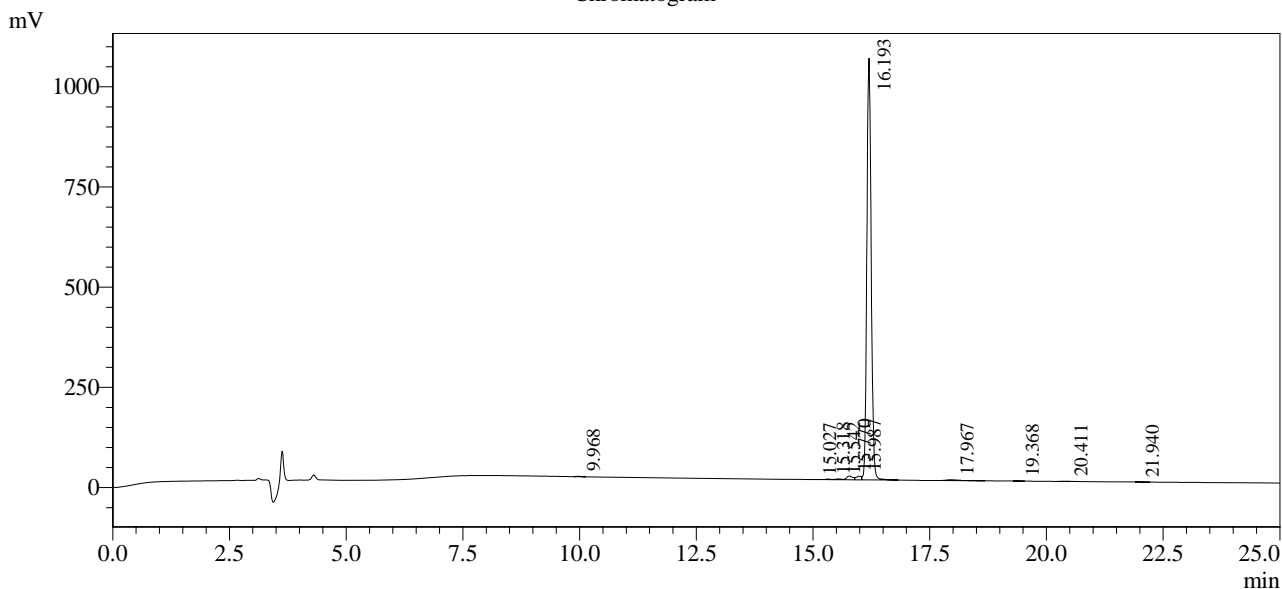

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.968	6077	1185	0.086
2	15.027	1110	155	0.016
3	15.318	9609	1298	0.136
4	15.542	16054	1868	0.227
5	15.770	84859	9233	1.202
6	15.987	68832	8943	0.975
7	16.193	6821746	1052118	96.647
8	17.967	42232	2130	0.598
9	19.368	1388	220	0.020
10	20.411	5499	412	0.078
11	21.940	1042	65	0.015
Total		7058447	1077626	100.000