

Sample Name :Thrombin Receptor Agonist  
Cat No.: RP10623  
Lot No.: E7001219J  
Time Processed :9:12:19  
Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
Equipment:ZJ19010324

### <Chromatogram>

mV

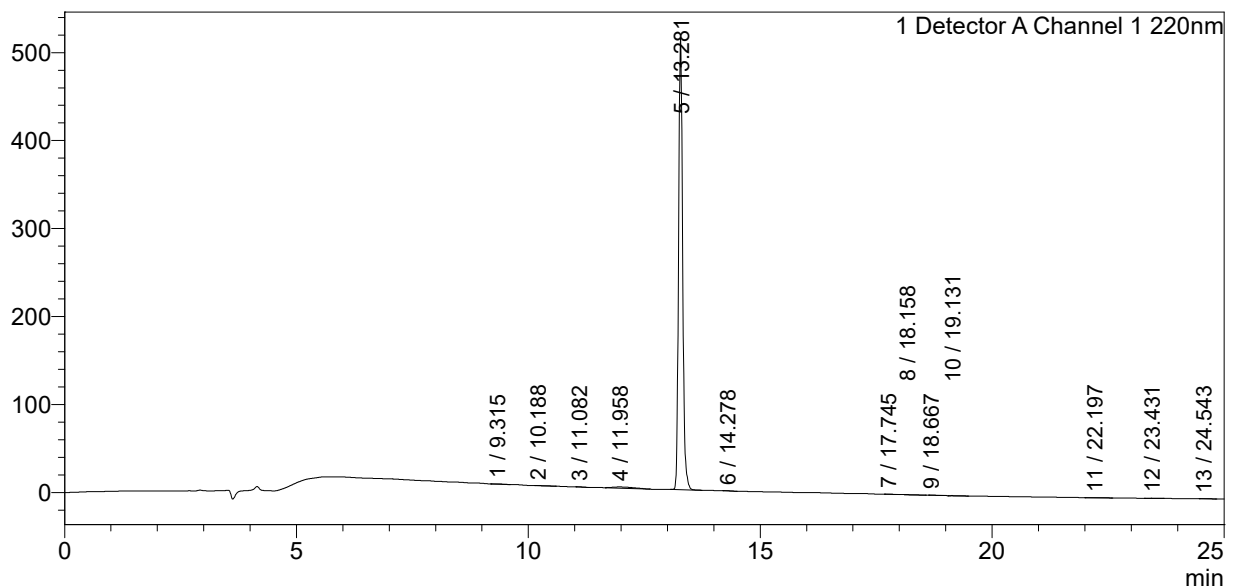

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.315	3515	287	0.109
2	10.188	1901	108	0.059
3	11.082	2320	138	0.072
4	11.958	46504	1378	1.443
5	13.281	3153248	513473	97.831
6	14.278	1989	298	0.062
7	17.745	1637	107	0.051
8	18.158	2719	158	0.084
9	18.667	1278	58	0.040
10	19.131	2058	104	0.064
11	22.197	2830	164	0.088
12	23.431	1659	136	0.051
13	24.543	1514	90	0.047
Total		3223172	516498	100.000