

Sample Name : Influenza NP (147-155)
 Cat. No. : RP20260
 Lot. No. : E6887820H
 Time Processed :8:02:37
 Month-Day-Year Processed :08/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

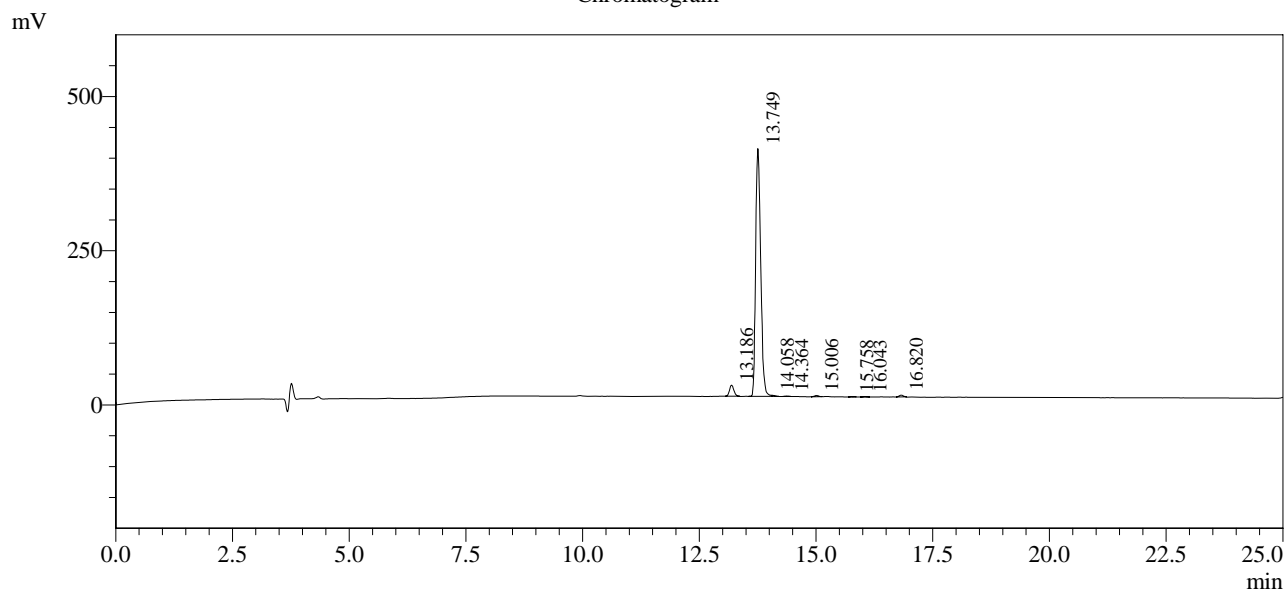

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.186	114545	17935	3.599
2	13.749	3025548	401675	95.067
3	14.058	6407	1768	0.201
4	14.364	2765	527	0.087
5	15.006	11836	1952	0.372
6	15.758	1232	276	0.039
7	16.043	2615	491	0.082
8	16.820	17589	2911	0.553
Total		3182536	427535	100.000