


Mass Spectrum

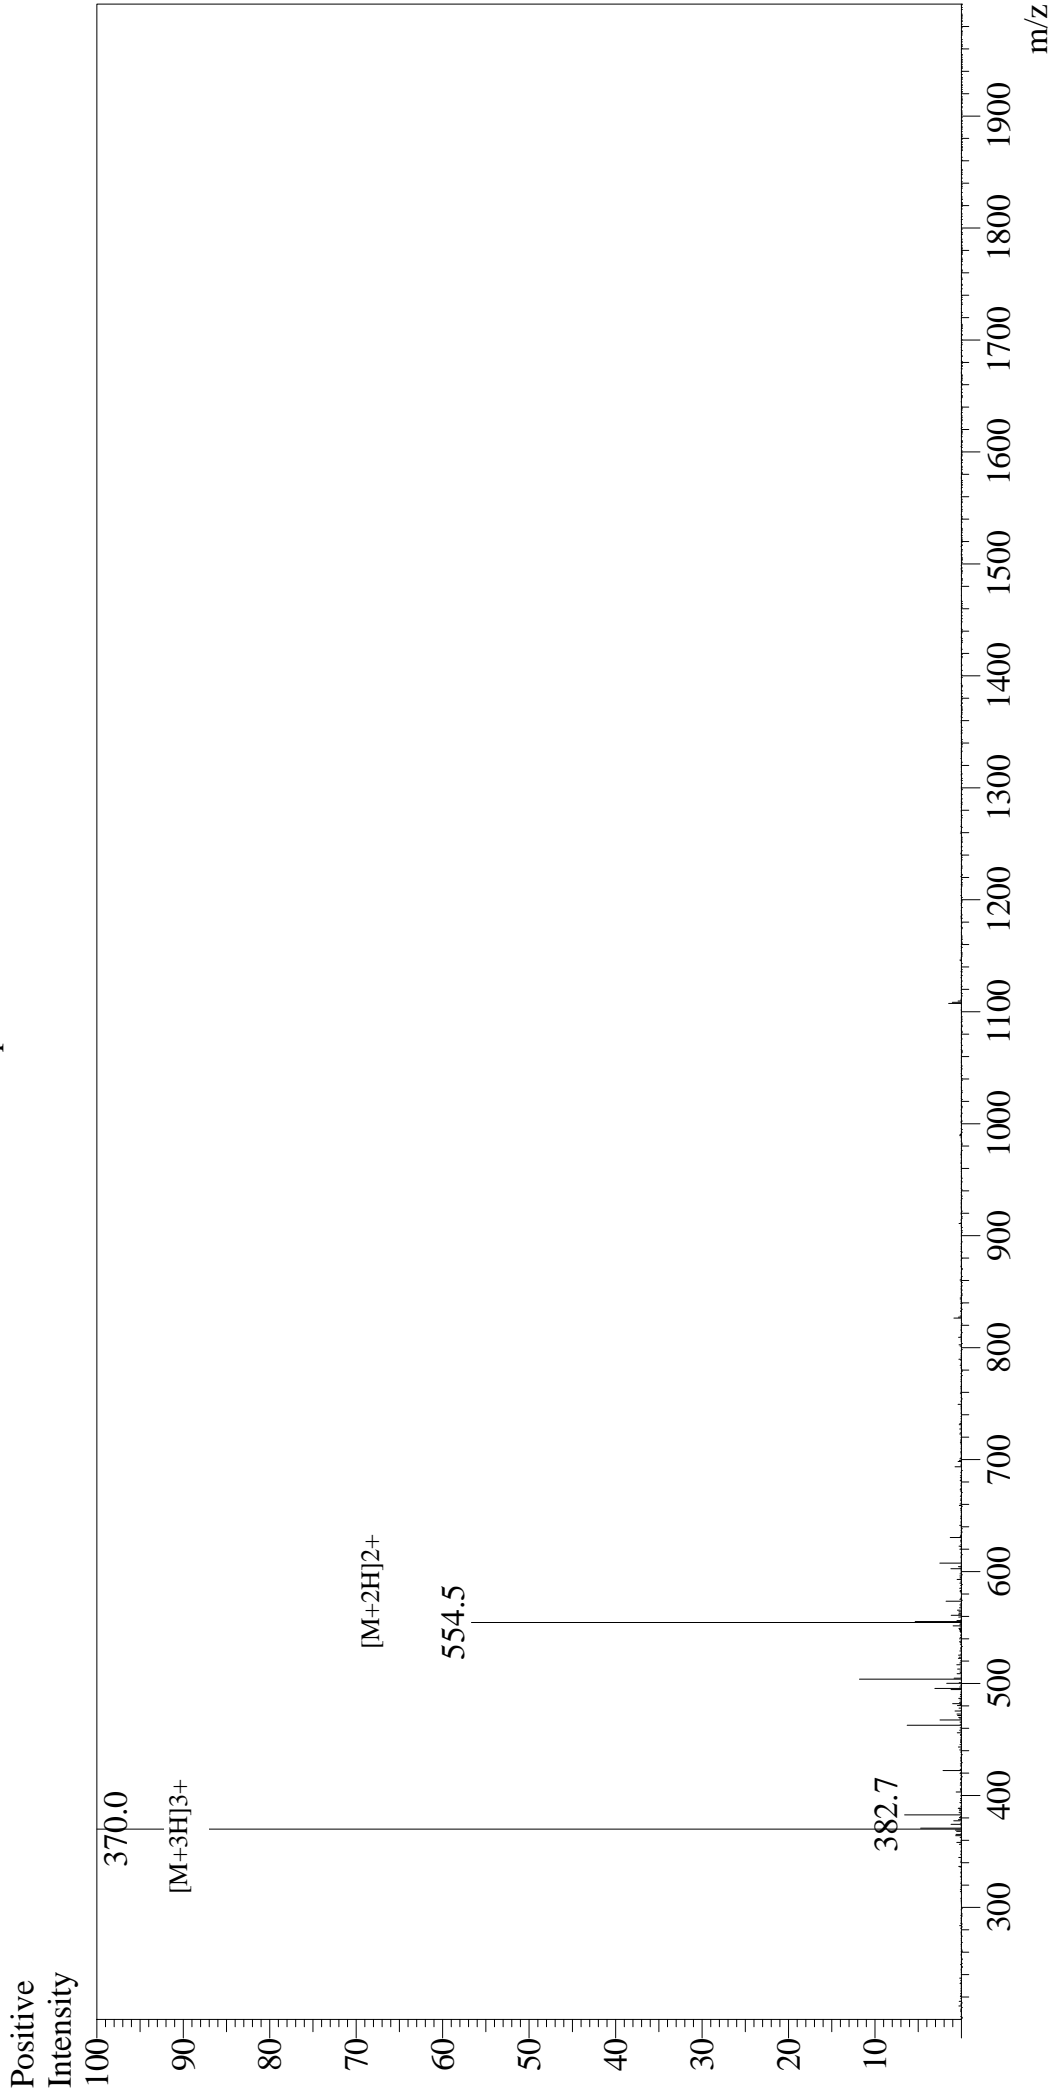

Sample Information
Month-Day Processed : 08/09/20
Time Processed : 8:20:57
Injection Volume : 0.3
Sample Name : Influenza NP (147-155)
Cat No. : RP20260
Lot No. : E6887820H
Theoretical MW : 1107.27
Observed MW : 1107.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH