

Sample Name :PAR2 AP
 Cat No. :RP19975
 Lot No. :PE6171905
 Time Processed :5:17:13
 Month-Day-Year Processed :05/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

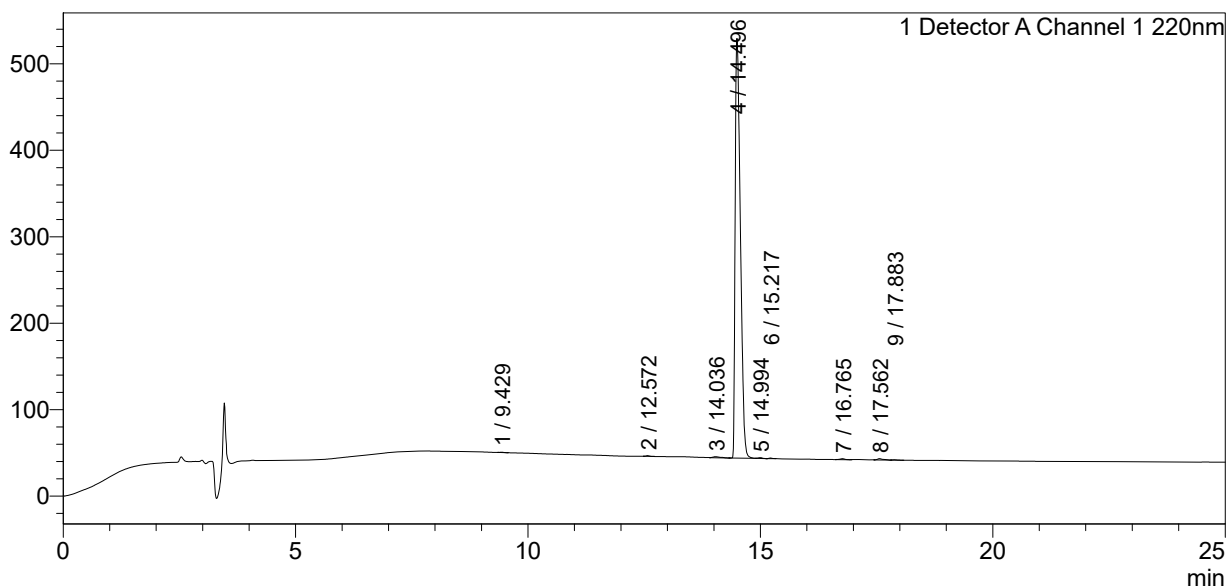

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.429	2309	432	0.060
2	12.572	3981	821	0.104
3	14.036	13004	1202	0.339
4	14.496	3785967	485209	98.707
5	14.994	5385	920	0.140
6	15.217	3204	674	0.084
7	16.765	7392	1061	0.193
8	17.562	12475	1477	0.325
9	17.883	1858	314	0.048
Total		3835575	492111	100.000