

Sample Name:[Met5]-Enkephalin
 Cat No.: RP10886
 Lot No.: E8979120J
 Time Processed :9:35:04
 Month-Day-Year Processed :11/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

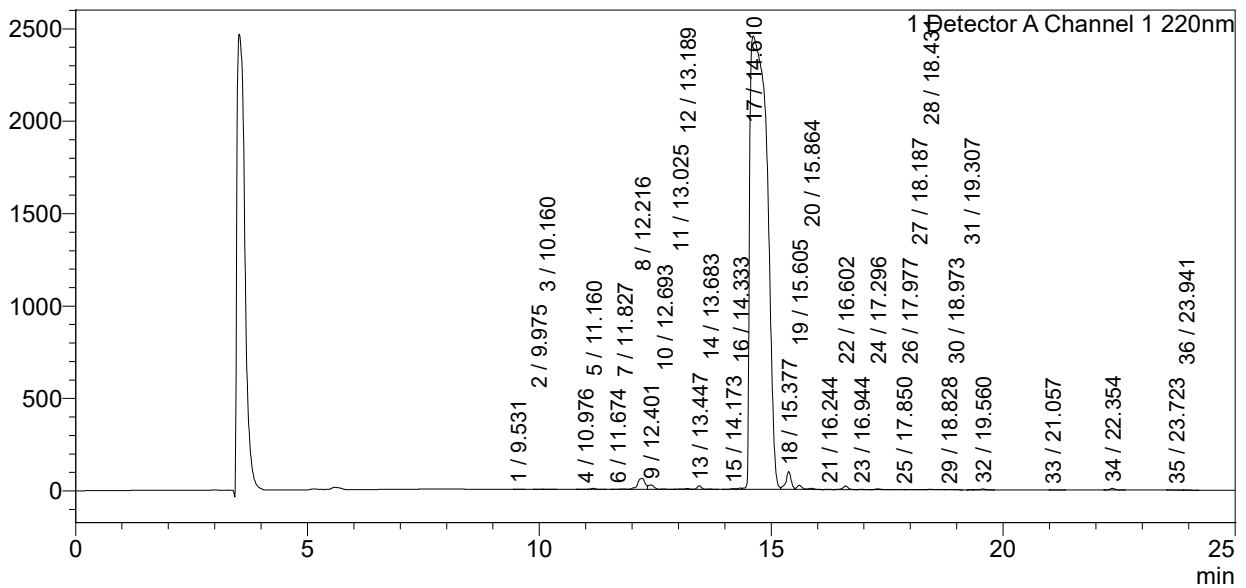

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.531	1444	217	0.002
2	9.975	1430	203	0.002
3	10.160	4954	606	0.008
4	10.976	2615	277	0.004
5	11.160	35395	5198	0.054
6	11.674	5732	831	0.009
7	11.827	14854	1696	0.023
8	12.216	672596	59910	1.028
9	12.401	206155	23954	0.315
10	12.693	14529	1943	0.022
11	13.025	16923	2755	0.026
12	13.189	33114	5091	0.051
13	13.447	133236	19655	0.204
14	13.683	14714	2031	0.022
15	14.173	32941	4121	0.050

Peak#	Ret. Time	Area	Height	Area%
16	14.333	45578	7191	0.070
17	14.610	62841433	2454229	96.069
18	15.377	765244	97689	1.170
19	15.605	166922	22577	0.255
20	15.864	51876	6313	0.079
21	16.244	2168	355	0.003
22	16.602	148424	19507	0.227
23	16.944	7666	1098	0.012
24	17.296	36896	4460	0.056
25	17.850	4503	615	0.007
26	17.977	9671	1146	0.015
27	18.187	10890	1235	0.017
28	18.431	16886	2221	0.026
29	18.828	3736	499	0.006
30	18.973	1923	317	0.003
31	19.307	1187	221	0.002
32	19.560	34497	4315	0.053
33	21.057	1843	237	0.003
34	22.354	64986	8489	0.099
35	23.723	4239	382	0.006
36	23.941	1583	174	0.002
Total		65412784	2761760	100.000