

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat  
 Cat No. : RP11095  
 Lot No. : E4998321F  
 Time Processed : 9:54:02 AM  
 Month-Day-Year Processed : 06/04/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

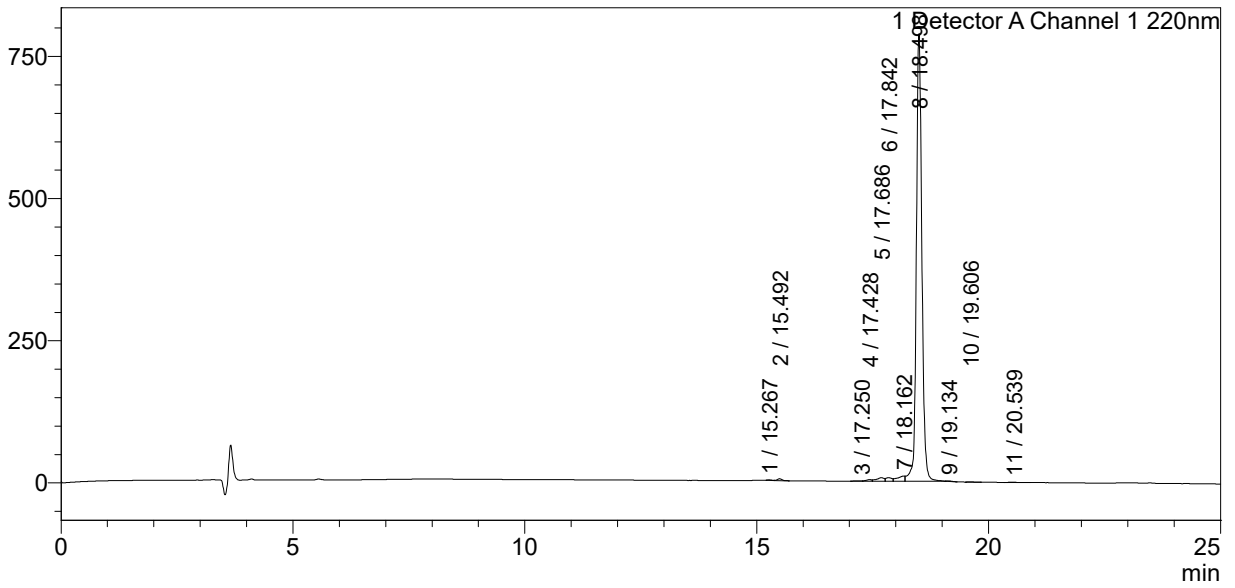

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.267	5930	1035	0.087
2	15.492	20952	3180	0.308
3	17.250	5898	615	0.087
4	17.428	22140	2562	0.325
5	17.686	69410	6047	1.020
6	17.842	55841	6206	0.821
7	18.162	103193	8907	1.517
8	18.498	6509004	786980	95.664
9	19.134	4983	739	0.073
10	19.606	2853	352	0.042
11	20.539	3840	266	0.056
Total		6804044	816888	100.000