

Sample Name :β-Amyloid (1-17)
 Cat. No. : RP20161
 Lot. No. : E4841119I
 Time Processed :13:46:04
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0286

Chromatogram

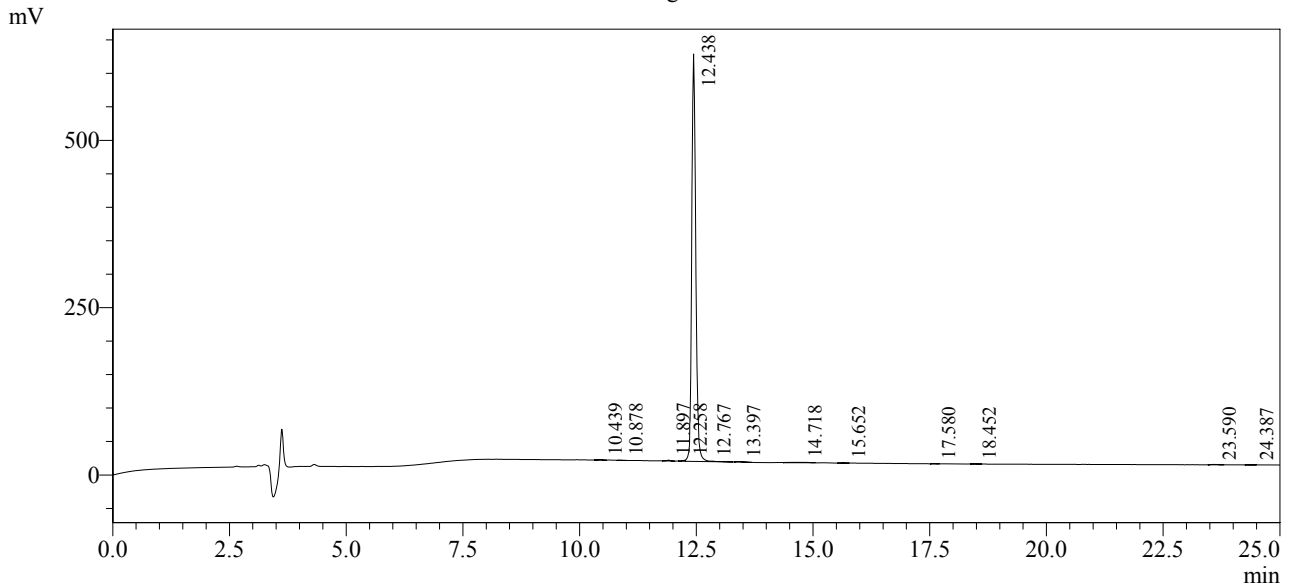

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.439	3423	634	0.092
2	10.878	1125	197	0.030
3	11.897	6768	1222	0.181
4	12.258	7196	1551	0.193
5	12.438	3664170	608775	98.256
6	12.767	10146	820	0.272
7	13.397	6941	781	0.186
8	14.718	19354	973	0.519
9	15.652	1077	150	0.029
10	17.580	1079	192	0.029
11	18.452	1479	248	0.040
12	23.590	5412	699	0.145
13	24.387	1032	115	0.028
Total		3729200	616357	100.000