

Sample Name :Orexin B, human
 Cat No.: RP10415
 Lot No.: E4811519I
 Time Processed:7:28:34
 Month-Day-Year Processed:09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

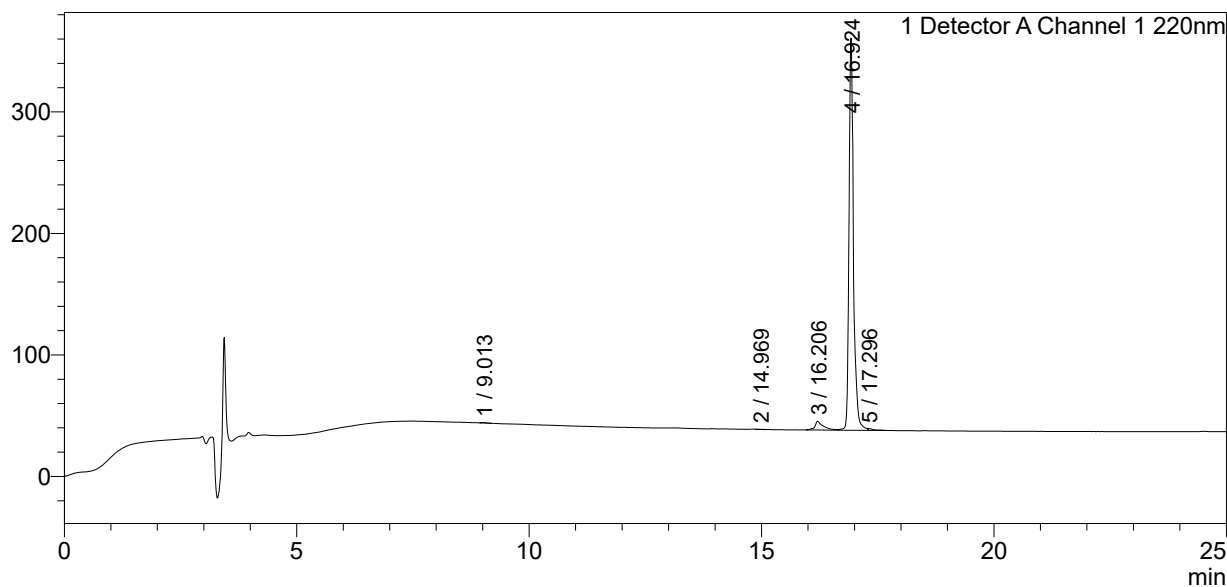

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.013	2002	373	0.089
2	14.969	1891	321	0.084
3	16.206	89244	7150	3.957
4	16.924	2148761	322750	95.277
5	17.296	13374	1516	0.593
Total		2255272	332109	100.000