

Sample Name :PLP(139-151)
 Cat. No. :RP10550
 Lot. No. :PE7141711

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

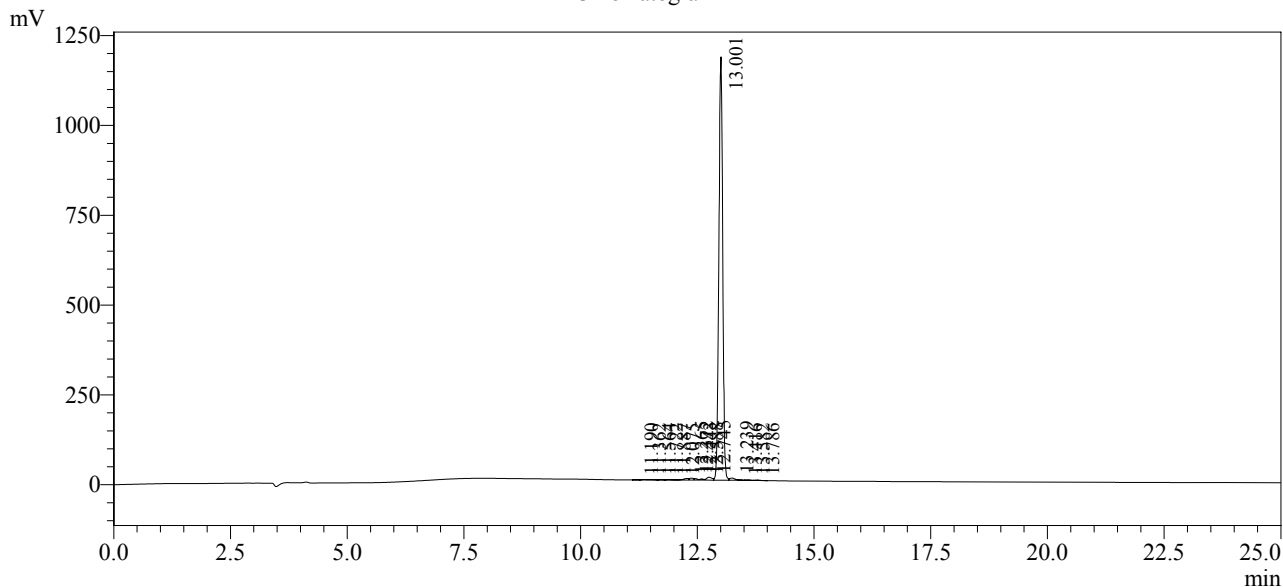

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.190	1233	223	0.017
2	11.362	8385	848	0.119
3	11.564	4330	677	0.061
4	11.722	6327	970	0.090
5	11.887	8981	1158	0.127
6	12.075	5825	917	0.083
7	12.265	33370	4527	0.473
8	12.372	33102	5504	0.469
9	12.443	18368	4035	0.260
10	12.588	17969	3291	0.255
11	12.745	65020	8062	0.922
12	13.001	6786384	1178195	96.180
13	13.239	47214	6170	0.669
14	13.416	5633	1162	0.080
15	13.582	5372	1008	0.076
16	13.786	8375	1404	0.119
Total		7055890	1218152	100.000