

Sample Name :  $\beta$ -Amyloid (1-40)  
 Cat. No. : RP10004  
 Lot. No. : E4686119I  
 Time Processed : 14:51:52  
 Month-Day-Year Processed : 10/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010009

Chromatogram

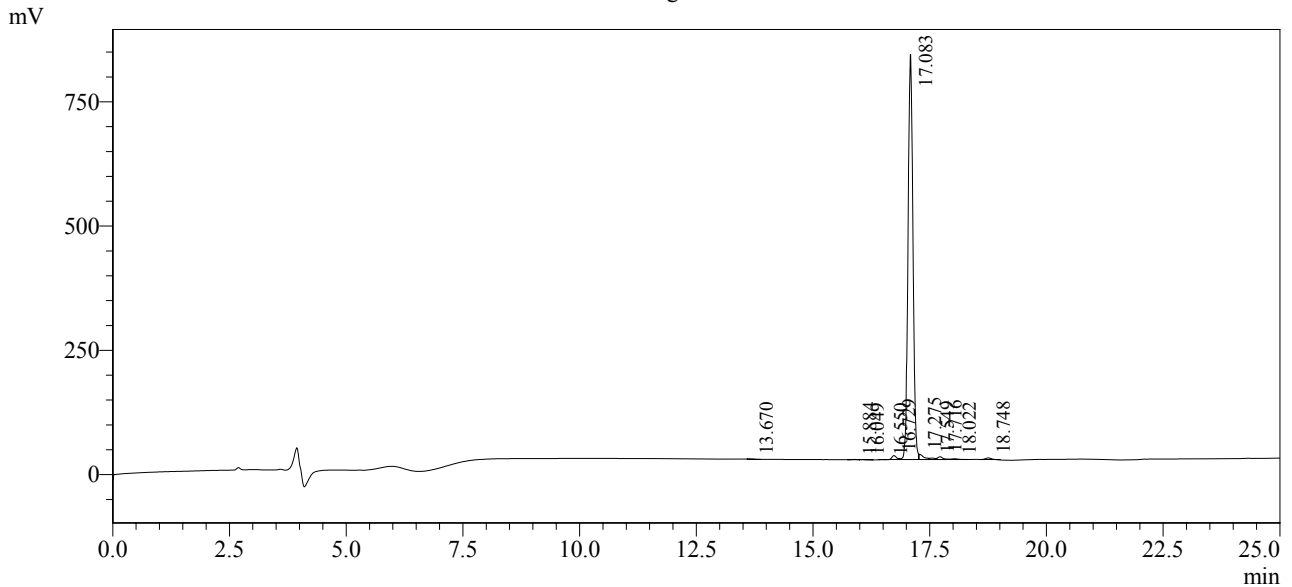

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.670	3799	599	0.061
2	15.884	4345	552	0.069
3	16.049	3389	486	0.054
4	16.550	1150	142	0.018
5	16.729	54306	8041	0.868
6	17.083	6010391	815072	96.024
7	17.275	72448	10503	1.157
8	17.549	25013	2898	0.400
9	17.716	41432	5517	0.662
10	18.022	16125	1418	0.258
11	18.748	26831	3225	0.429
Total		6259229	848454	100.000