

Sample Name :Exendin-4
 Cat. No. : RP10874
 Lot. No. : E0090319L
 Time Processed :0:03:14
 Month-Day-Year Processed : 12/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

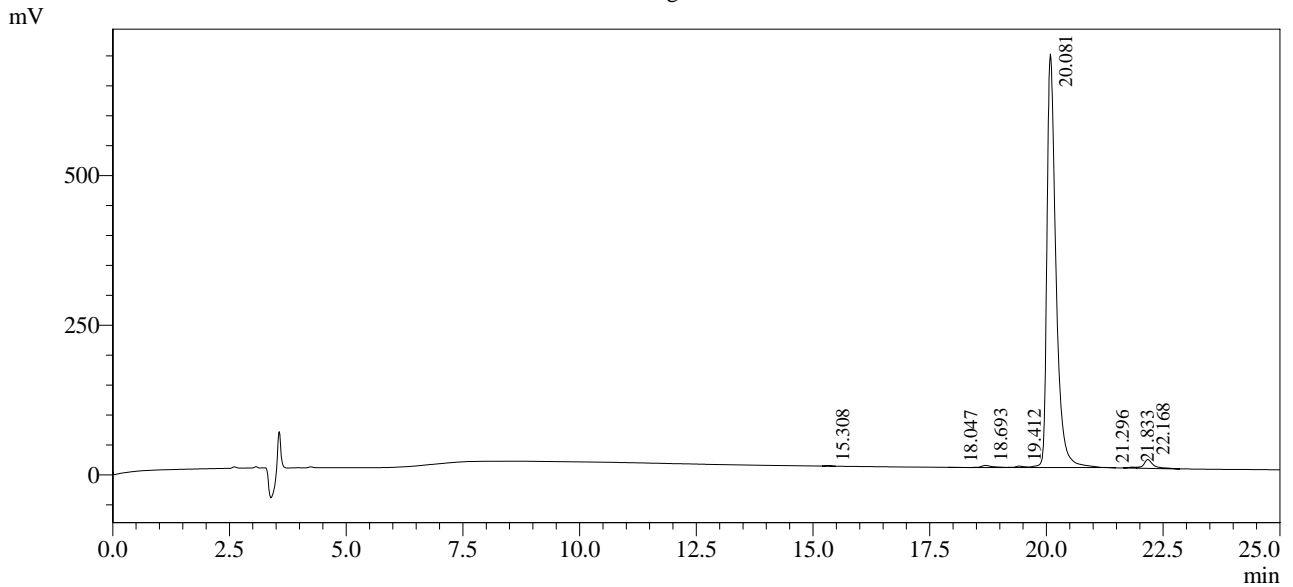

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.308	5687	853	0.059
2	18.047	3528	445	0.037
3	18.693	55994	3438	0.581
4	19.412	28708	2338	0.298
5	20.081	9302869	690959	96.576
6	21.296	3005	404	0.031
7	21.833	19901	1707	0.207
8	22.168	213038	14883	2.212
Total		9632731	715026	100.000