

Sample Name: NP (396-404)
 Cat No. : RP20090
 Lot. No. : E5465519L
 Time Processed: 5:03:32 PM
 Month-Day-Year Processed : 12/06/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

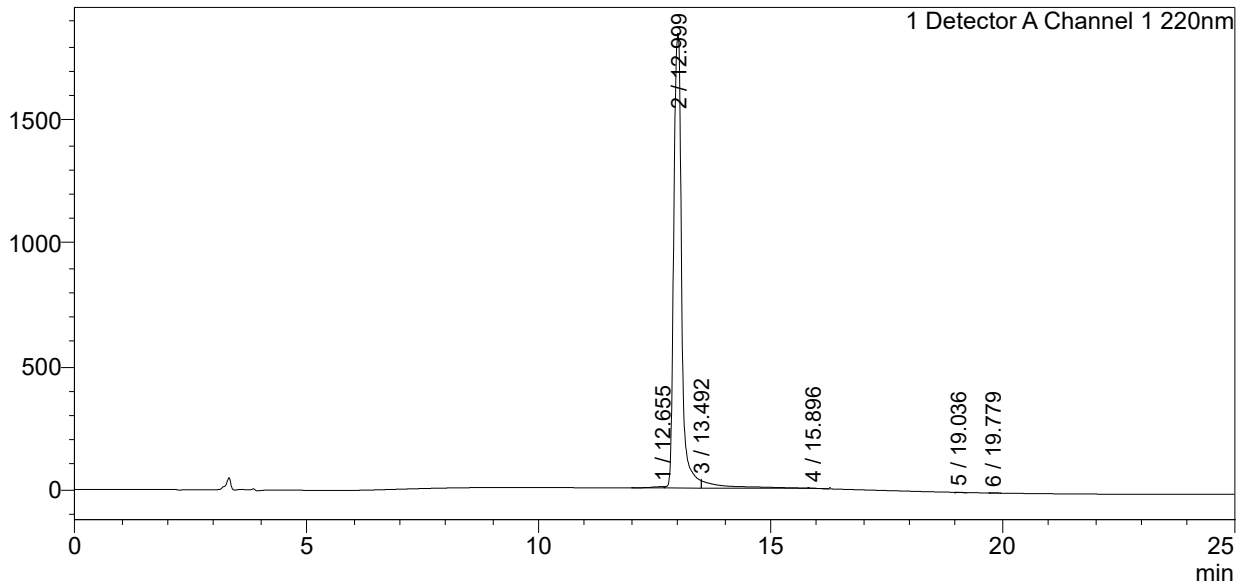

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.655	107609	6104	0.475
2	12.999	2155504	1849158	95.244
3	13.492	954232	31397	4.216
4	15.896	8491	832	0.038
5	19.036	2470	394	0.011
6	19.779	3521	546	0.016
Total		22631827	1888430	100.000