

Sample Name :RGD
 Cat. No. : RP20297
 Lot. No. :PE5501712

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

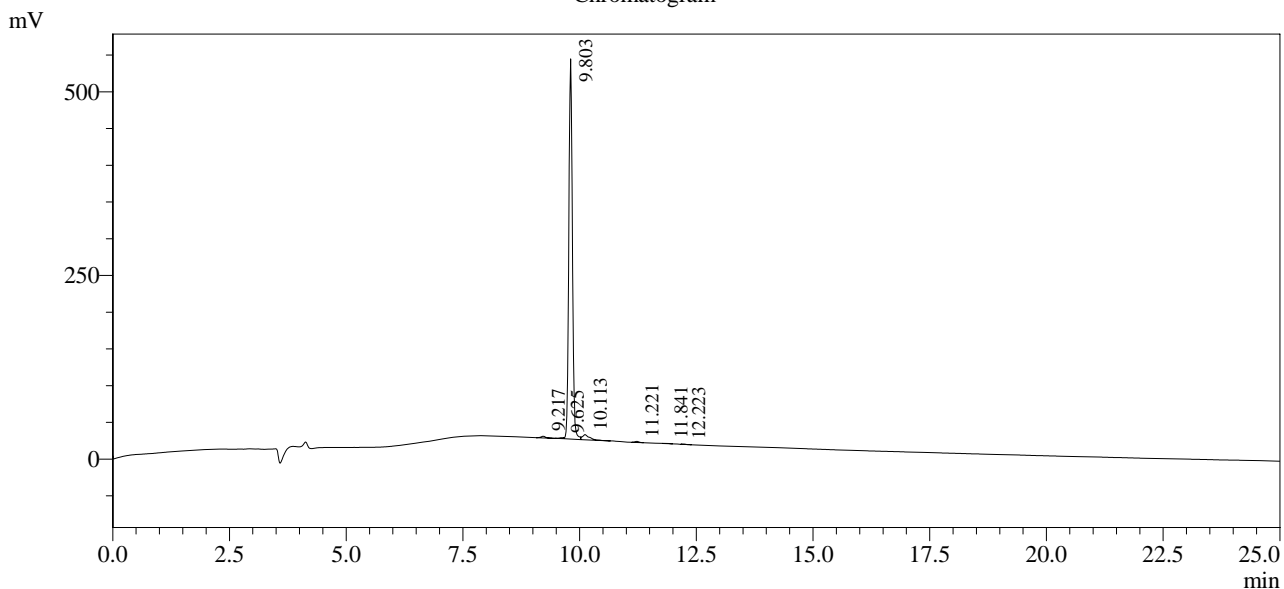

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.217	15756	2190	0.548
2	9.625	8447	1353	0.294
3	9.803	2761674	517525	96.108
4	10.113	74343	6960	2.587
5	11.221	8689	1426	0.302
6	11.841	2790	488	0.097
7	12.223	1826	403	0.064
Total		2873525	530346	100.000