

Sample Name :Bradykinin (1-7)
 Cat No. :RP11133
 Lot No. :E1699519J
 Time Processed :21:07:46
 Month-Day-Year Processed :10/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

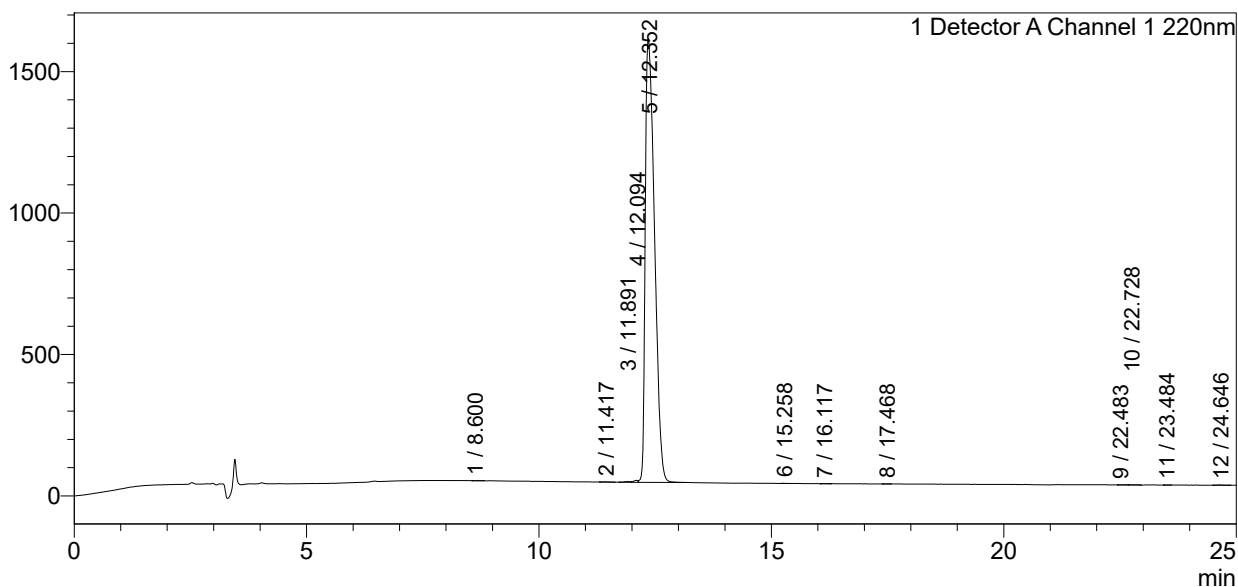

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.600	1766	222	0.008
2	11.417	6636	579	0.030
3	11.891	21842	2304	0.100
4	12.094	43078	6792	0.197
5	12.352	21777922	1568633	99.571
6	15.258	2625	451	0.012
7	16.117	2199	292	0.010
8	17.468	1300	287	0.006
9	22.483	2068	200	0.009
10	22.728	3906	496	0.018
11	23.484	1296	255	0.006
12	24.646	7189	865	0.033
Total		21871829	1581376	100.000