

Sample Name :InsB 9-23  
 Cat. No. : RP20391  
 Lot. No. : PE8831902  
 Time Processed : 9:14:39  
 Month-Day-Year Processed : 03/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

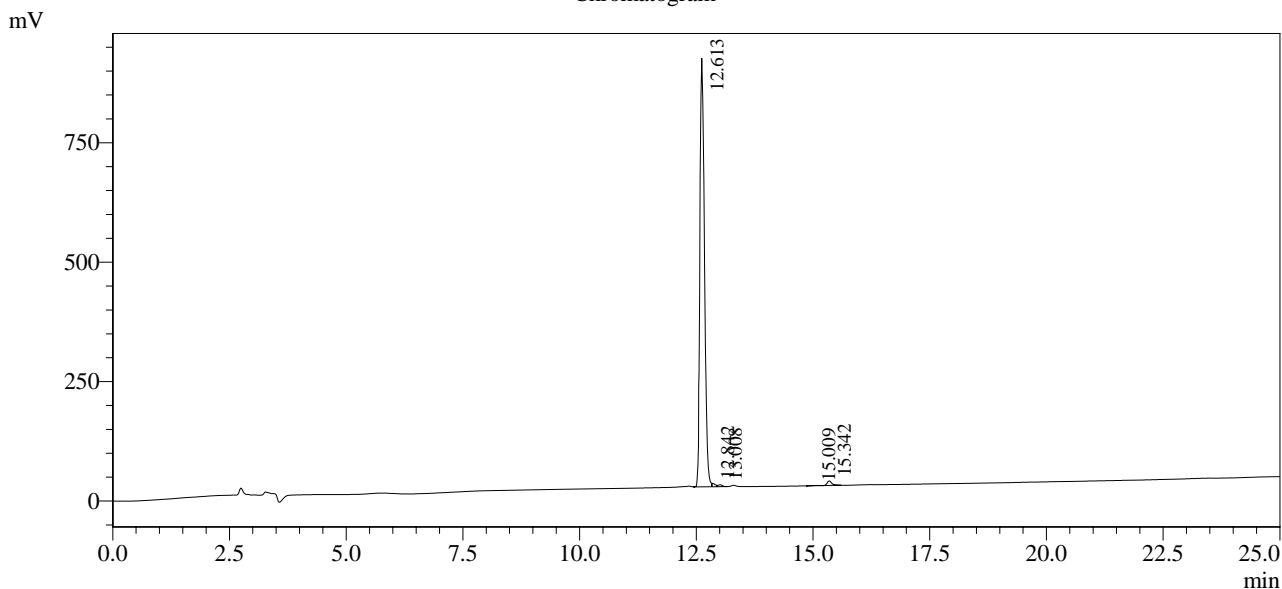

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.613	6136897	897083	98.000
2	12.842	33192	6809	0.530
3	13.008	23770	3772	0.380
4	15.009	5876	716	0.094
5	15.342	62424	9423	0.997
Total		6262158	917802	100.000