

Sample Name : M2e,human  
 Cat. No. : RP20206  
 Lot. No. : PE4421611


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

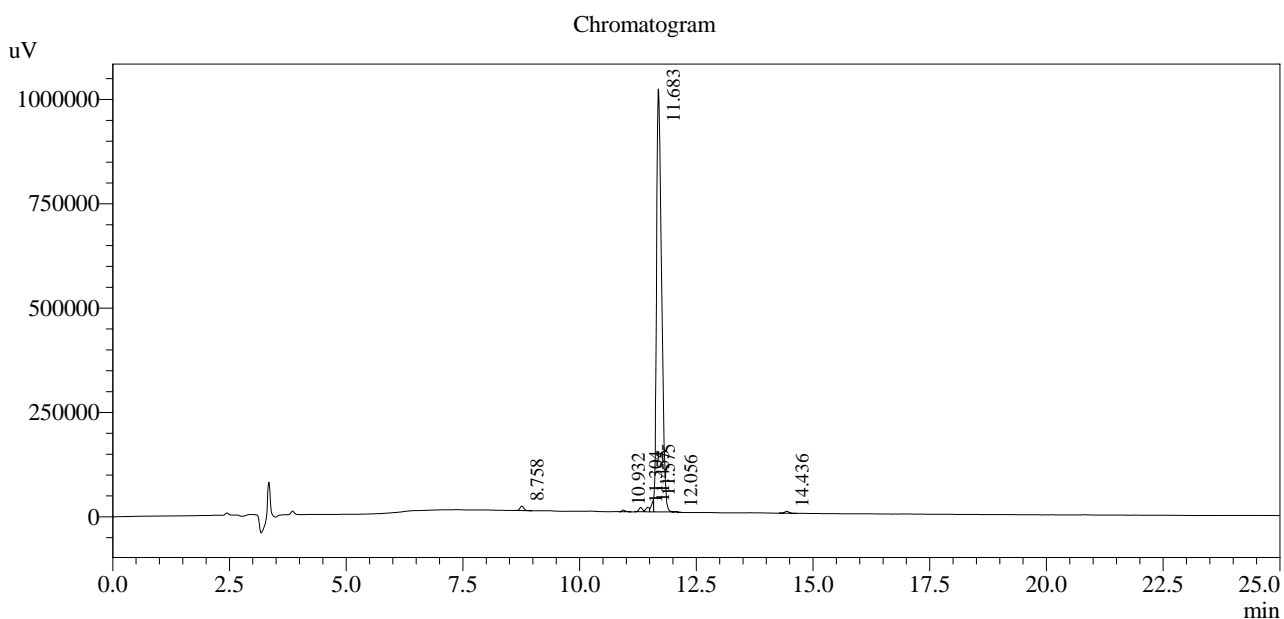

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.758	61126	10774	0.768
2	10.932	19168	3968	0.241
3	11.304	56919	10486	0.715
4	11.455	55344	10920	0.695
5	11.575	91274	27006	1.146
6	11.683	7640821	1013762	95.964
7	12.056	5376	1211	0.068
8	14.436	32175	4726	0.404
Total		7962202	1082853	100.000