

Sample Name :Gastrin-1, human
 Cat. No. : RP12740
 Lot. No. : E5666921C
 Time Processed : 9:39:12 AM
 Month-Day-Year Processed : 04/08/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

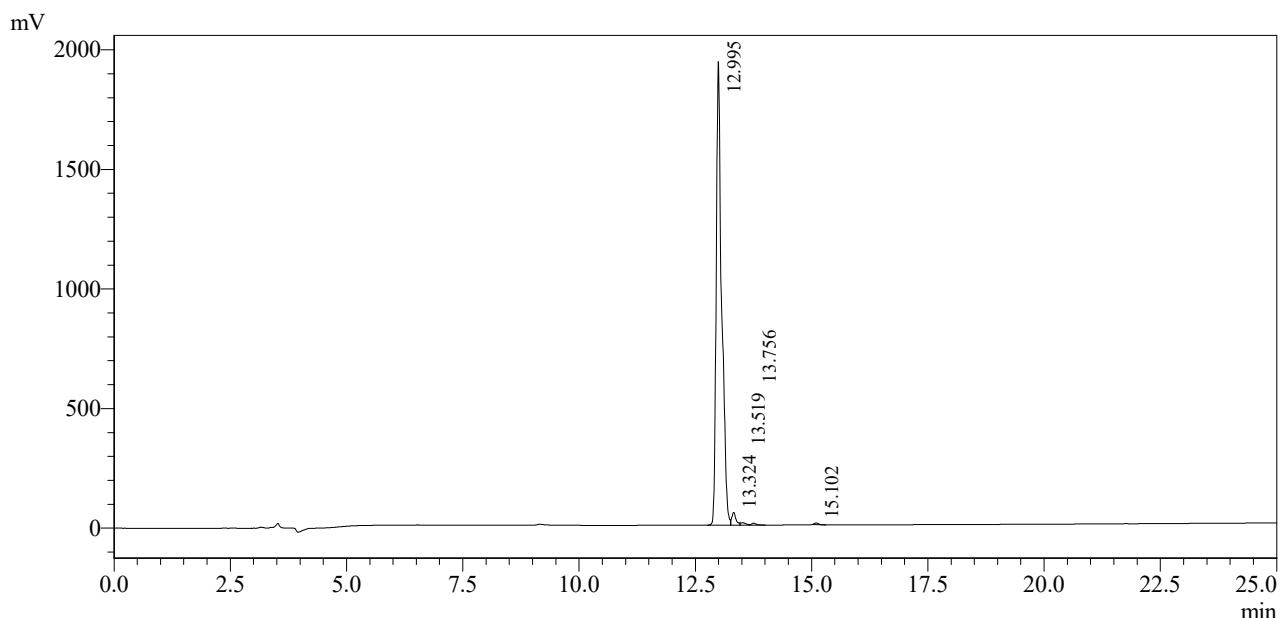

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.995	15758047	1937469	96.885
2	13.324	332469	53264	2.044
3	13.519	77466	9670	0.476
4	13.756	55642	8065	0.342
5	15.102	41012	6824	0.252
Total		16264636	2015293	100.000