

Sample Name : (Arg)9
 Cat No.: RP20403
 Lot No.: E6546520B
 Time Processed : 9:41:23
 Month-Day-Year Processed : 02/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
41.00	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

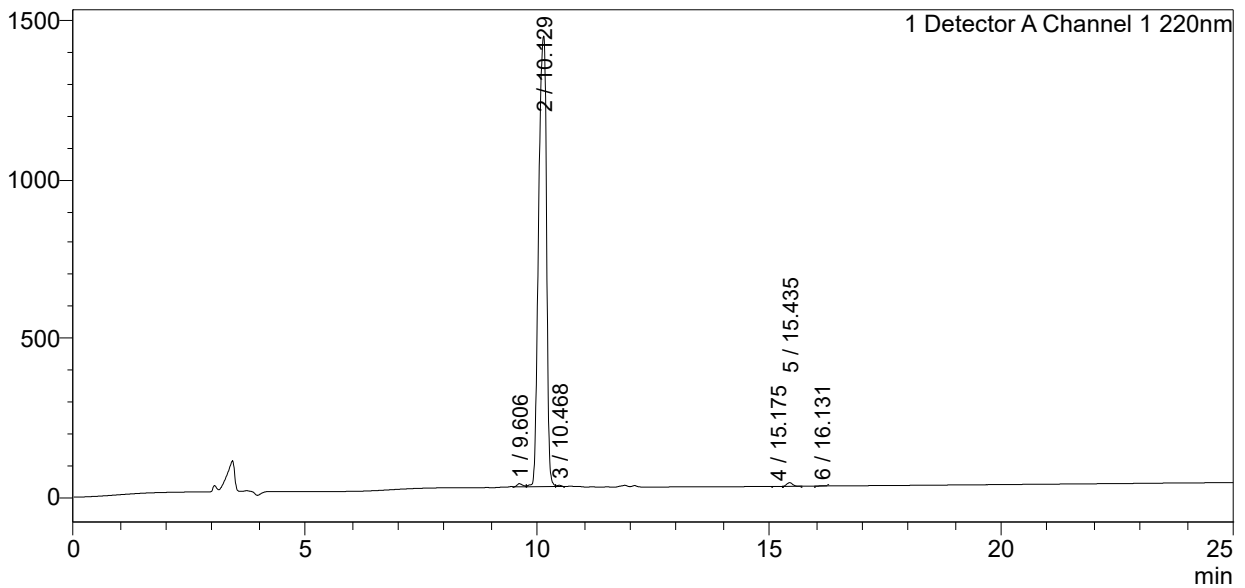

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.606	80794	9596	0.476
2	10.129	16746778	1418601	98.737
3	10.468	25248	4080	0.149
4	15.175	1592	195	0.009
5	15.435	102679	11626	0.605
6	16.131	3885	564	0.023
Total		16960976	1444663	100.000