

Sample Name : Kemptide  
 Cat. No. : RP10287  
 Lot. No. : E4709019I  
 Time Processed :3:12:50  
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	20	
40.00	Pumps	Pump A B.Conc	20	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

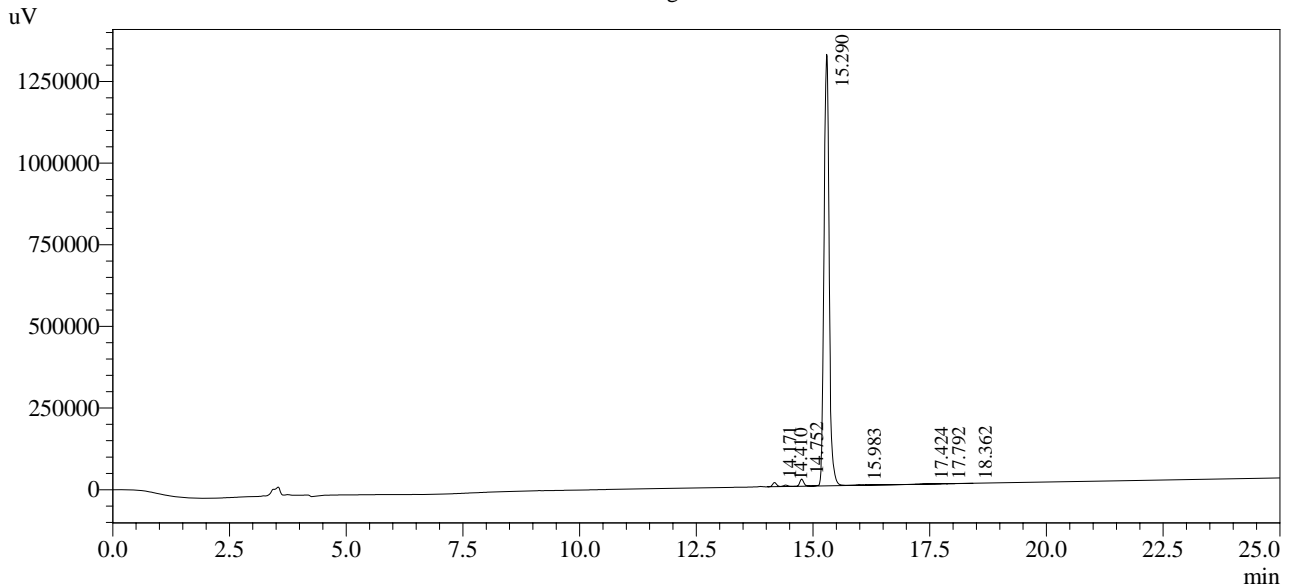

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.171	76228	12803	0.726
2	14.410	29432	4311	0.280
3	14.752	134912	21804	1.286
4	15.290	10226346	1321448	97.441
5	15.983	13529	1217	0.129
6	17.424	9763	885	0.093
7	17.792	2436	363	0.023
8	18.362	2280	128	0.022
Total		10494926	1362958	100.000