

Sample Name : Proctolin
 Cat. No. : RP10475
 Lot. No. : PE2011702


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : UniPS 10-300 10µm 4.6 x 250 mm

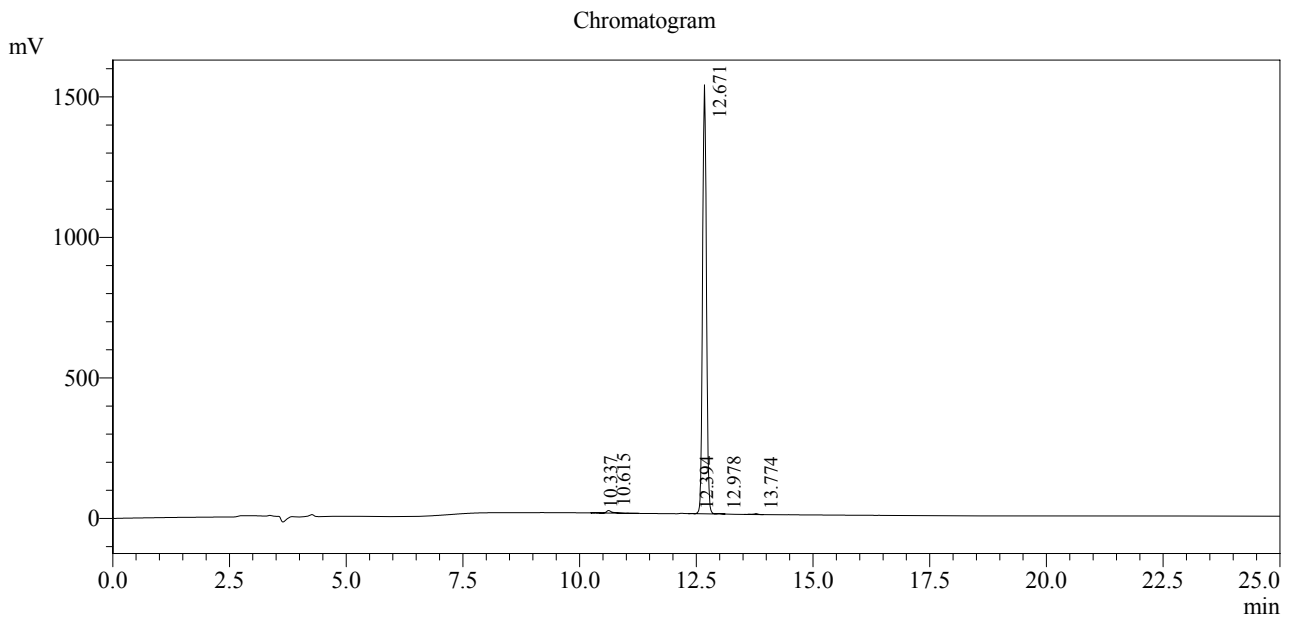

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.337	4410	697	0.049
2	10.615	79897	9178	0.891
3	12.394	2918	822	0.033
4	12.671	8847862	1526388	98.632
5	12.978	11215	1741	0.125
6	13.774	24264	3179	0.270
Total		8970566	1542005	100.000