

Sample Name :[Met5]-Enkephalin
 Cat. No. : RP10886
 Lot. No. :E4768119I
 Time Processed :11:14:35
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01 | Pumps | Pump B Conc. | 5 | |
| 25.00 | Pumps | Pump B Conc. | 65 | |
| 25.01 | Pumps | Pump B Conc. | 95 | |
| 27.00 | Pumps | Pump B Conc. | 95 | |
| 27.01 | Pumps | Pump B Conc. | 5 | |
| 35.00 | Pumps | Pump B Conc. | 5 | |
| 35.01 | Controller | Stop | | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

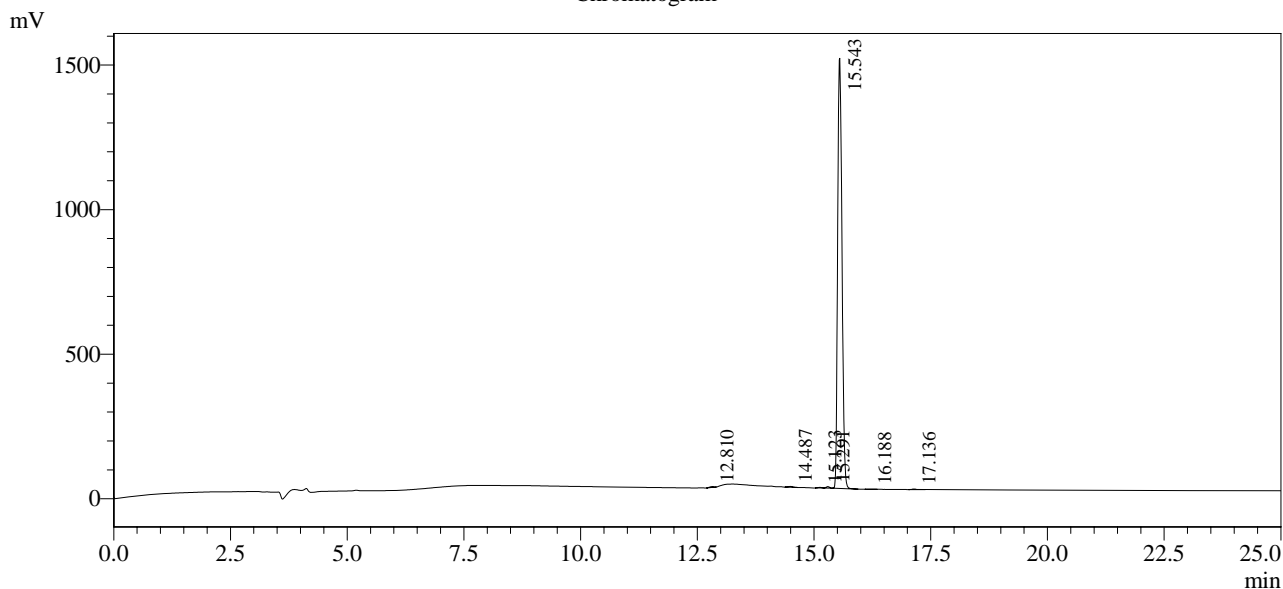

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|---------|---------|
| 1 | 12.810 | 18520 | 2948 | 0.191 |
| 2 | 14.487 | 19274 | 2767 | 0.198 |
| 3 | 15.123 | 10140 | 2005 | 0.104 |
| 4 | 15.291 | 26287 | 5206 | 0.270 |
| 5 | 15.543 | 9631795 | 1487965 | 99.072 |
| 6 | 16.188 | 4296 | 718 | 0.044 |
| 7 | 17.136 | 11727 | 2116 | 0.121 |
| Total | | 9722039 | 1503724 | 100.000 |