

Sample Name:Urotensin II, human
 Cat No.:RP10096
 Lot No.:E2776720E
 Time Processed :2:42:52
 Month-Day-Year Processed :06/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 15 |
| 25.00 | Pumps | Pump A B.Conc | 75 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 30.00 | Pumps | Pump A B.Conc | 95 |
| 30.01 | Pumps | Pump A B.Conc | 15 |
| 35.00 | Pumps | Pump A B.Conc | 15 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

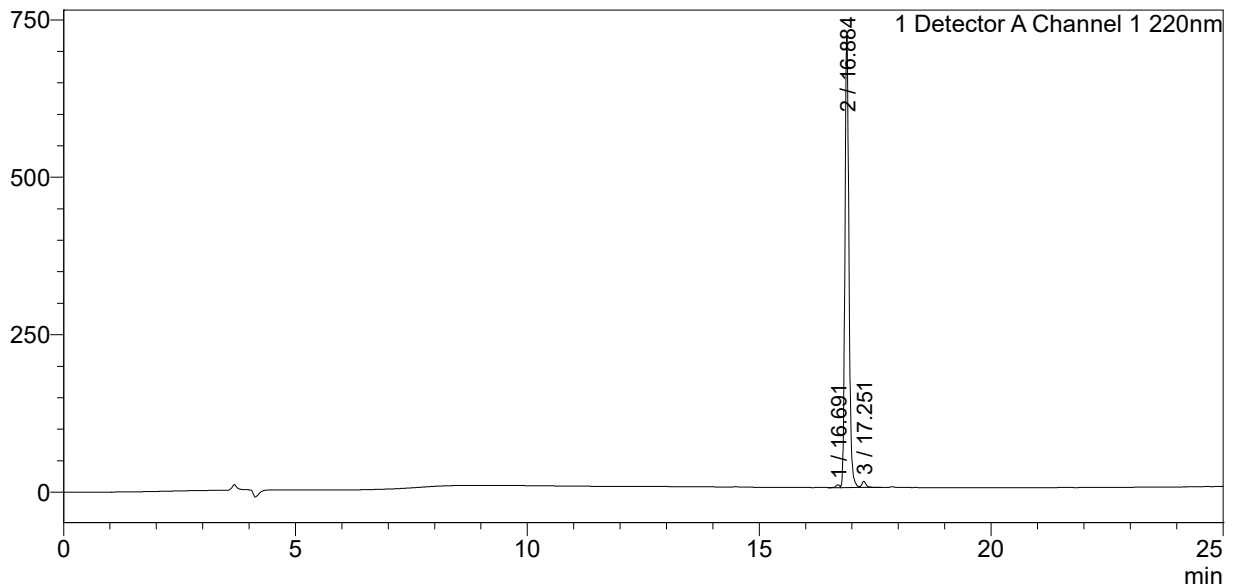

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 16.691 | 24016 | 4362 | 0.542 |
| 2 | 16.884 | 4344976 | 717260 | 97.991 |
| 3 | 17.251 | 65075 | 9790 | 1.468 |
| Total | | 4434067 | 731413 | 100.000 |