

Sample Name : β -Amyloid (35-42)
 Cat No: RP20145
 Lot No: E4713320K
 Time Processed :8:20:59 AM
 Month-Day-Year Processed :11/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

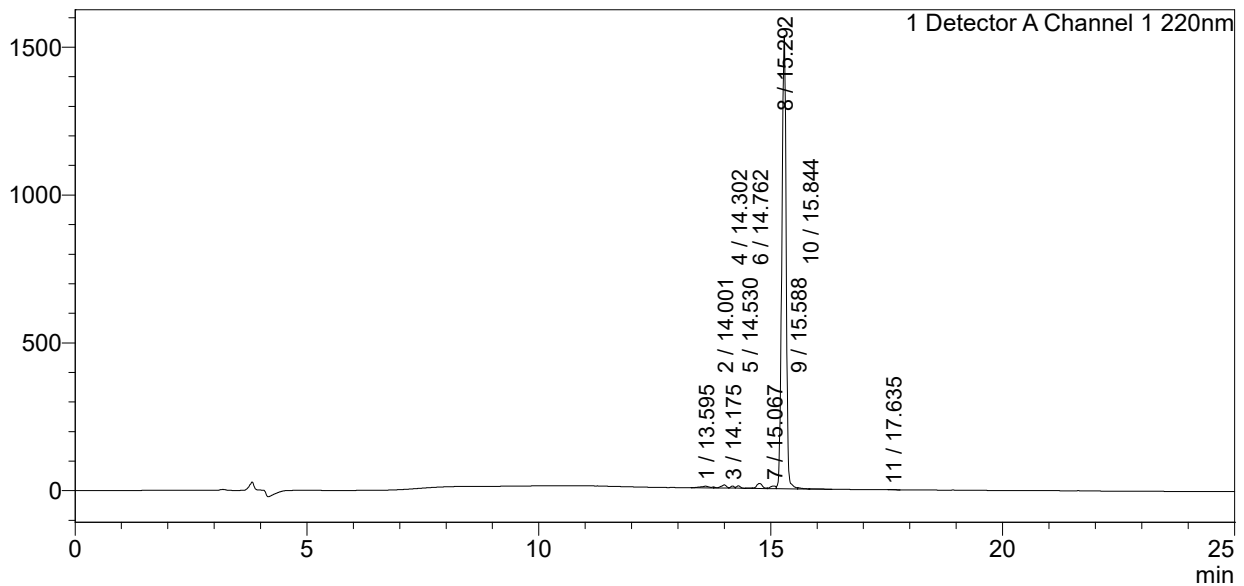

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.595	75635	5522	0.724
2	14.001	89974	10997	0.861
3	14.175	36002	7269	0.345
4	14.302	46056	8174	0.441
5	14.530	9746	1404	0.093
6	14.762	145600	16953	1.394
7	15.067	68708	8628	0.658
8	15.292	9940293	1533008	95.152
9	15.588	23122	4058	0.221
10	15.844	6215	534	0.059
11	17.635	5382	926	0.052
Total		10446733	1597474	100.000