

Sample Name :Fibronectin CS1 Peptide
 Cat No. : RP10838 Lot No. : PE1591807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

<Chromatogram>

mV

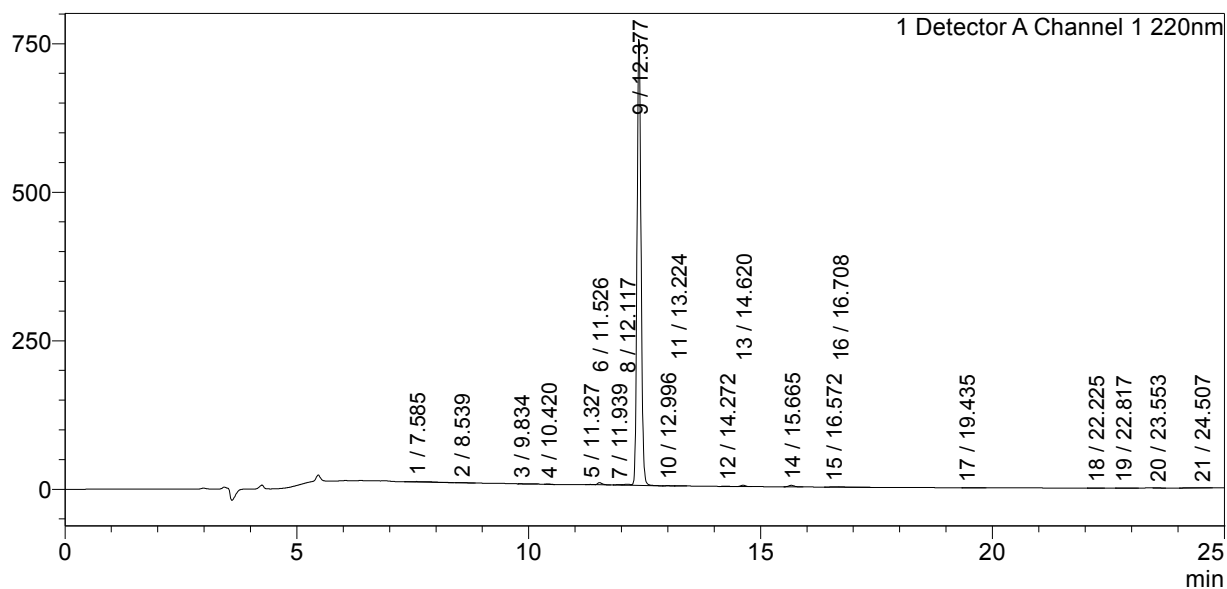

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.585	26347	734	0.559
2	8.539	3432	274	0.073
3	9.834	1820	107	0.039
4	10.420	4045	768	0.086
5	11.327	3138	516	0.067
6	11.526	25712	3866	0.546
7	11.939	7579	1058	0.161
8	12.117	16443	1840	0.349
9	12.377	4555434	751108	96.695
10	12.996	3150	496	0.067
11	13.224	1286	145	0.027
12	14.272	1941	191	0.041
13	14.620	16027	2346	0.340
14	15.665	20704	2525	0.439
15	16.572	6341	538	0.135
16	16.708	9550	489	0.203
17	19.435	1324	106	0.028
18	22.225	1244	89	0.026
19	22.817	1832	120	0.039

Peak#	Ret. Time	Area	Height	Area%
20	23.553	1362	121	0.029
21	24.507	2404	137	0.051
Total		4711113	767573	100.000