

Sample Name :Glucagon-Like Peptide (GLP) II, human
 Cat No. :RP10769
 Lot No. :E4543920H
 Time Processed :20:24:52
 Month-Day-Year Processed :08/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
41.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

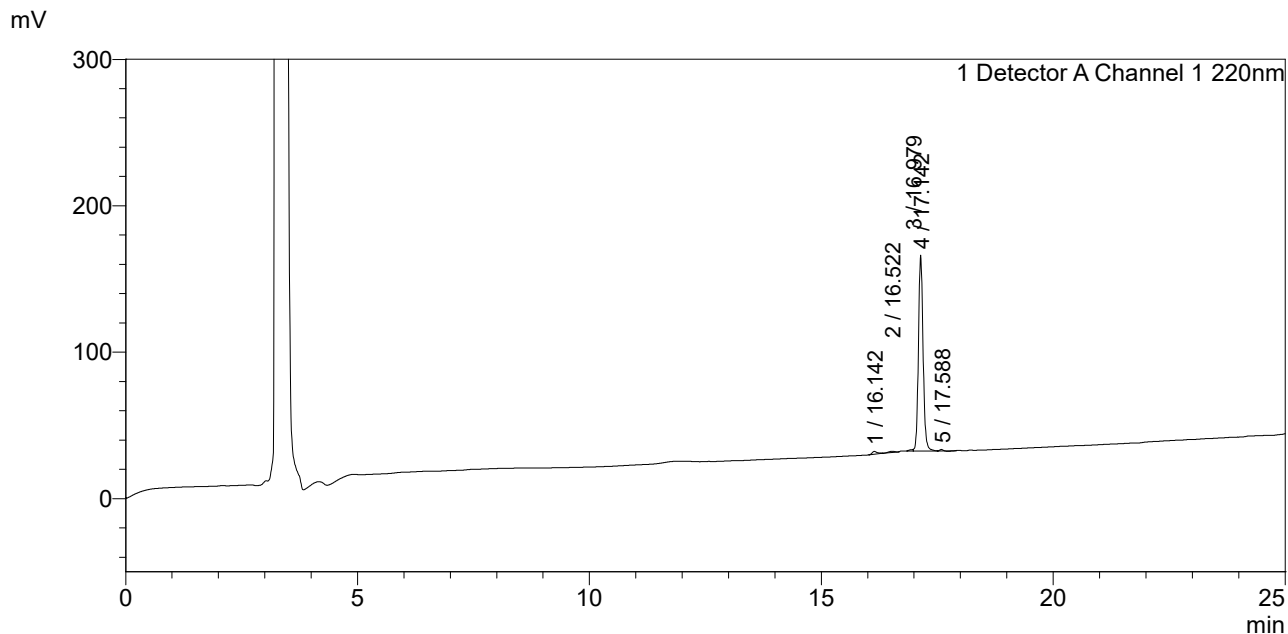

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.142	14447	1934	1.506
2	16.522	5930	678	0.618
3	16.979	5304	971	0.553
4	17.142	932742	133617	97.264
5	17.588	561	901	0.058
Total		958983	138100	100.000