

Sample Name :BNP(1-45), mouse
 Cat No.: RP20365
 Lot No.: E0104119L
 Time Processed :15:52:38
 Month-Day-Year Processed :01/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	15
25.00	Pumps	Solvent B Conc.	75
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	15
40.00	Pumps	Solvent B Conc.	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

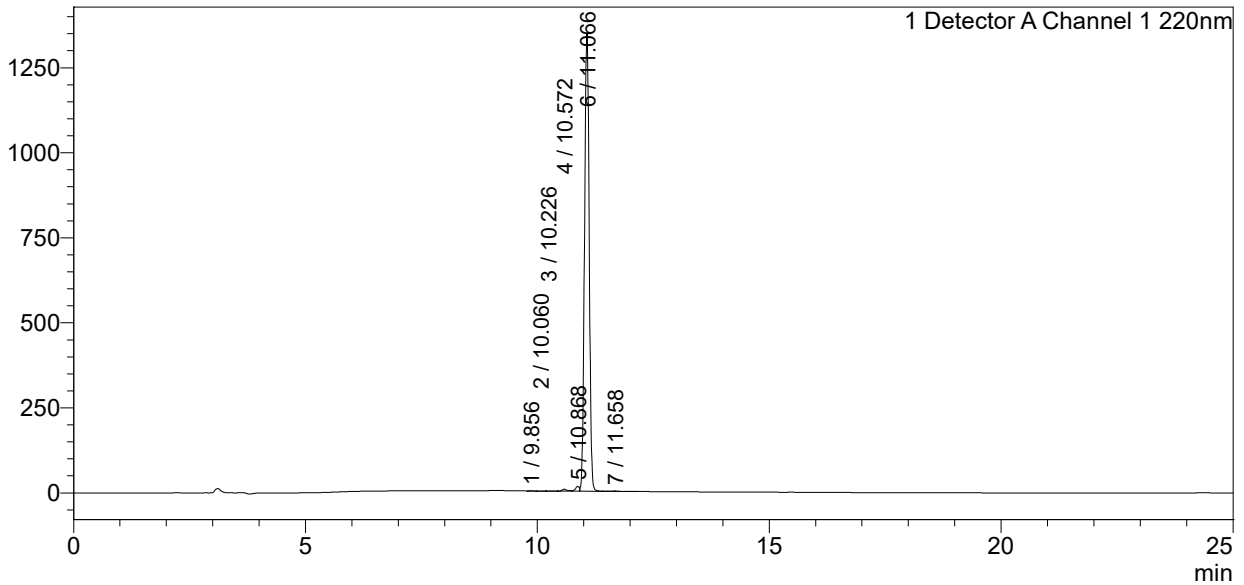

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.856	2669	562	0.028
2	10.060	1450	240	0.015
3	10.226	1422	122	0.015
4	10.572	46845	5888	0.485
5	10.868	87147	14182	0.902
6	11.066	9493250	1347878	98.289
7	11.658	25690	1485	0.266
Total		9658473	1370357	100.000