

Sample Name: Brain Natriuretic Peptide (BNP) (1-32), human
 Cat No. : RP11119
 Lot No. : E3431220B
 Time Processed: 3:50:05 PM
 Month-Day-Year Processed :02/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

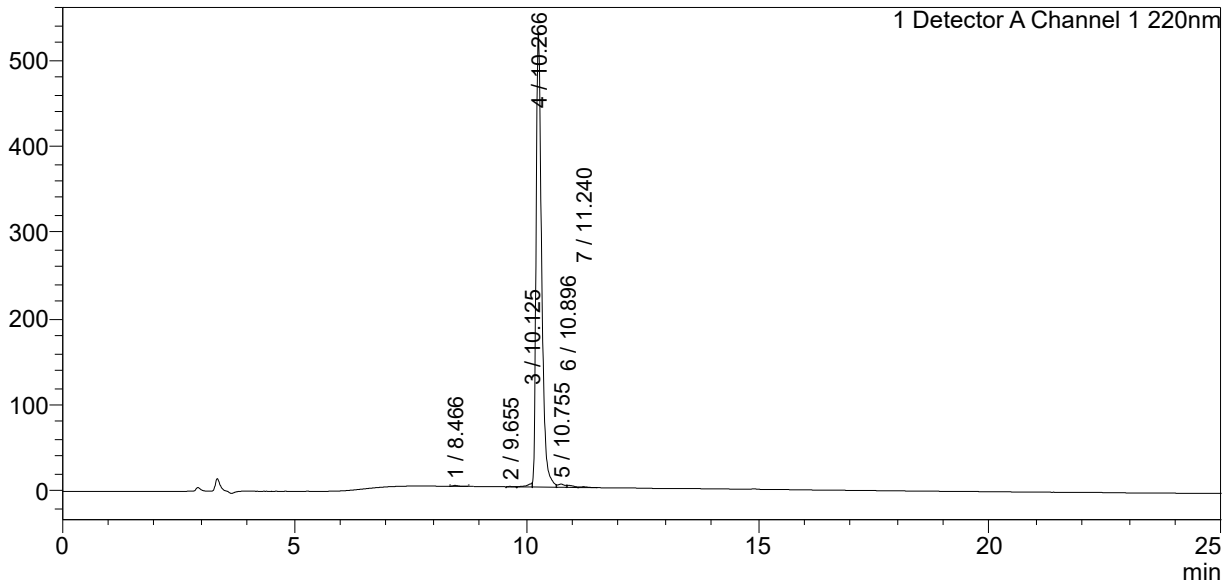

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.466	4503	907	0.100
2	9.655	3449	473	0.077
3	10.125	31418	3835	0.698
4	10.266	4391678	527679	97.523
5	10.755	32718	3783	0.727
6	10.896	28428	2447	0.631
7	11.240	11039	947	0.245
Total		4503233	540071	100.000