

Sample Name:N-Acetyl-Ser-Asp-Lys-Pro

Cat. No. : RP10555

Lot. No. : E3609219K

Time Processed: 18:02:38

Month-Day-Year Processed :11/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Equipment:ZJ19010324

### <Chromatogram>

mV

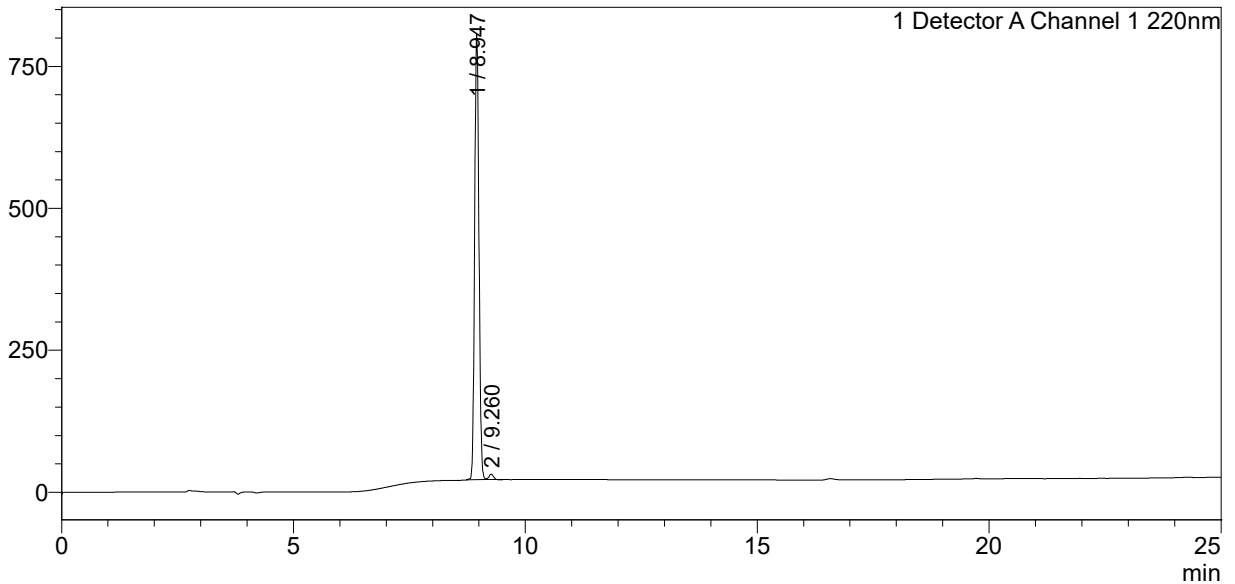

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.947	5097644	786606	98.809
2	9.260	61468	9636	1.191
Total		5159112	796243	100.000