


Mass Spectrum

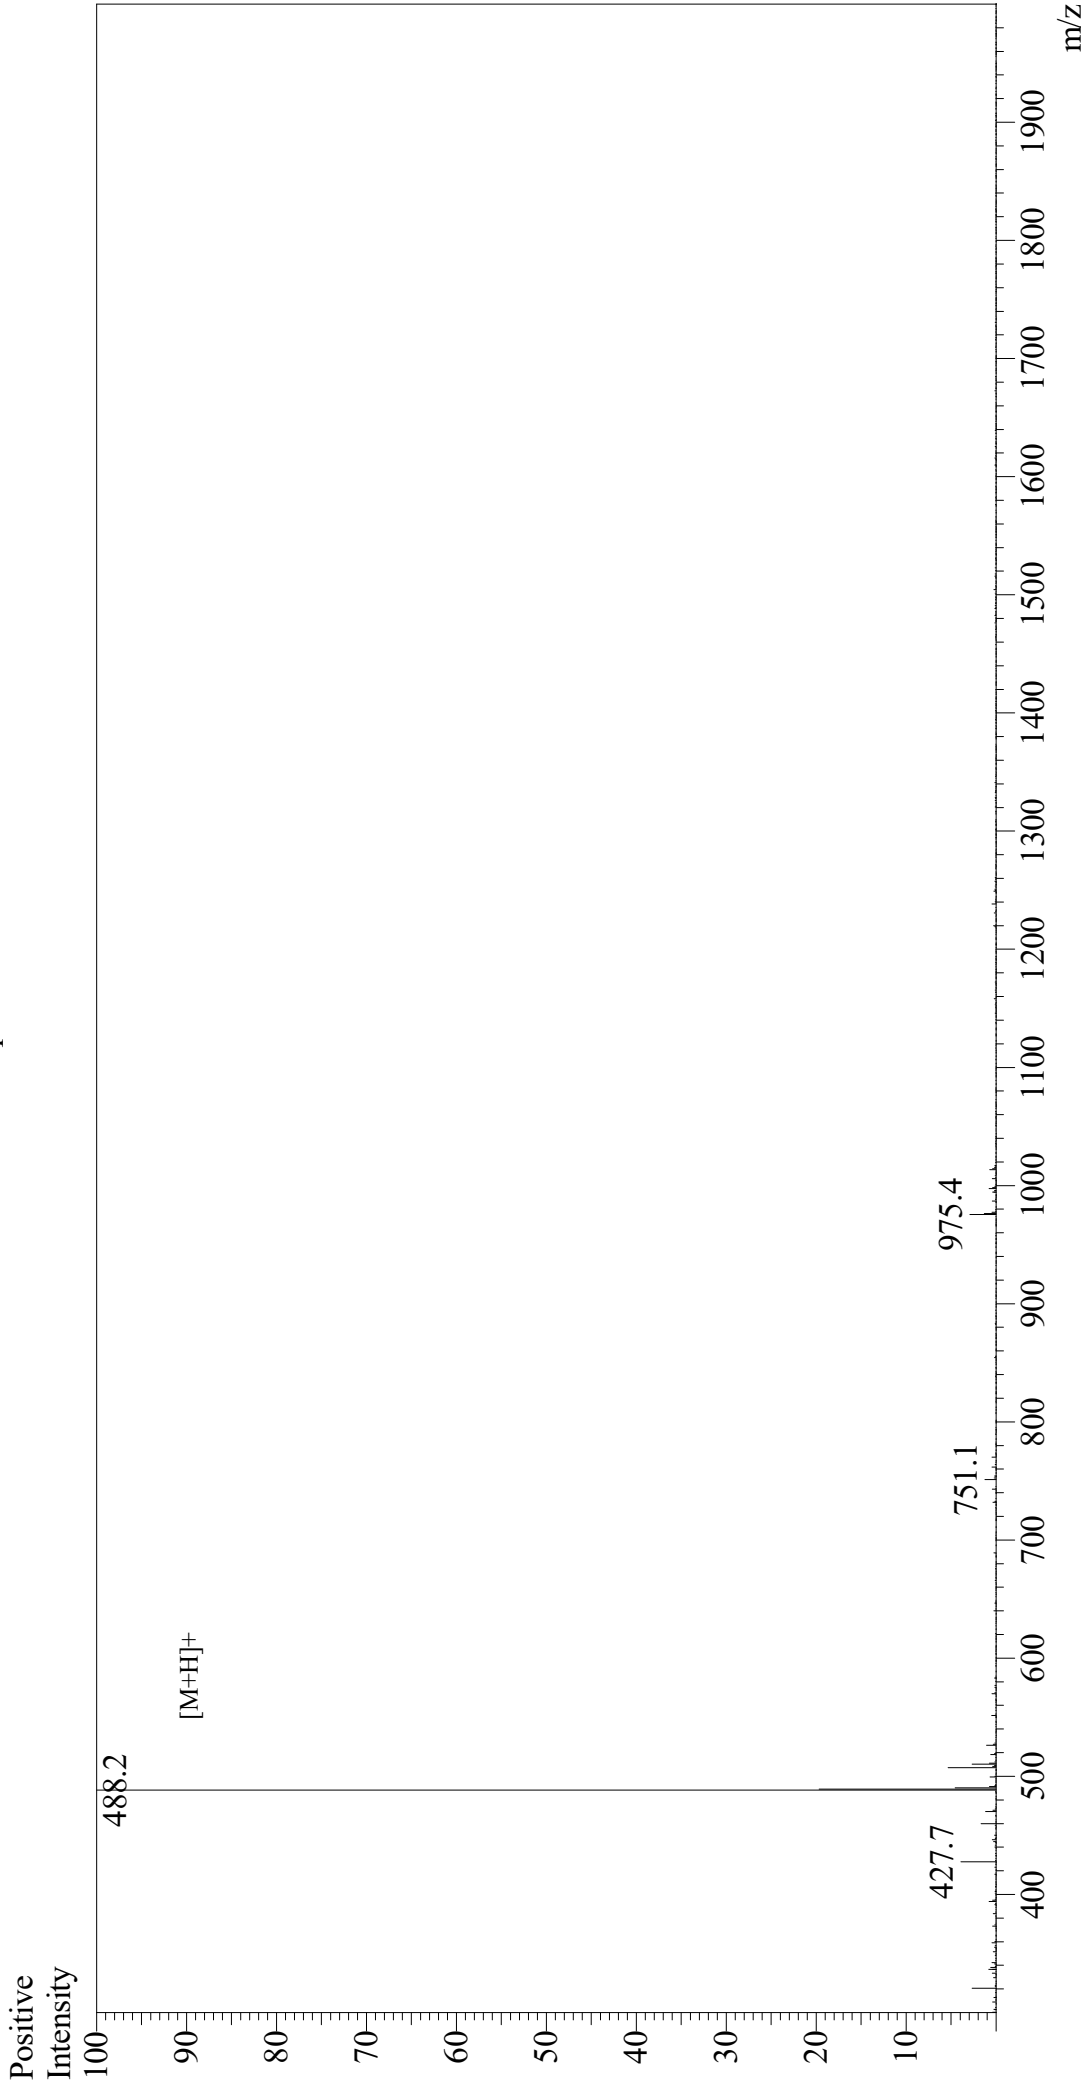

Sample Information

Acquired by: Gary
Month-Day Processed: 11/18/19
Time Processed: 10:04:30 AM
Injection Volume: 0.3
Sample Name: N-Acetyl-Ser-Asp-Lys-Pro
Cat. No.: RP10555
Lot. No.: E3609219K
Theoretical MW: 487.50
Observed MW: 487.2

Equipment: GK11010007
Interface Bias: +4.5 kV
Drying Gas Flow: 5 L/min
T.Flow: 0.2 ml/min
B.conc: 50% H2O/50% MeOH

Interface: ESI
Nebulizing Gas Flow: 1.5 L/min
CDL Temp: 250
Block Temp: 200